

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018868.D
 Acq On : 15 Dec 2023 06:00
 Operator : MA/JU
 Sample : 05627-14
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC6

Quant Time: Dec 15 06:29:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	234555	20.000	ng/u1	0.00
20) Naphthalene-d8	10.622	136	822787	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	463232	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	1074926	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1252011	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	1426334	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	26728	3.883	ng/uL	0.00
4) Pyridine-d5	3.681	84	129866	7.044	ng/u1	0.00
7) Phenol-d5	6.999	99	133736	5.682	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	318823	22.853	ng/u1	0.00
11) 2-Chlorophenol-d4	7.358	132	335185	18.249	ng/u1	0.00
15) 4-Methylphenol-d8	8.540	113	220225	11.561	ng/u1	0.00
21) Nitrobenzene-d5	8.993	128	185830	25.376	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	179398	23.629	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	358092	23.066	ng/u1	0.00
31) 4-Chloroaniline-d4	10.763	131	345406	17.024	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	1213157	29.343	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	1289927	28.334	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	43552	6.417	ng/u1	0.00
60) Fluorene-d10	15.451	176	1078896	31.089	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	146744	22.768	ng/u1	0.00
73) Anthracene-d10	17.304	188	1886139	33.377	ng/u1	0.00
81) Pyrene-d10	19.545	212	2494081	25.591	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.498	264	2539403	30.534	ng/u1	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.181	149	12993504	188.149	ng/u1#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018868.D
Acq On : 15 Dec 2023 06:00
Operator : MA/JU
Sample : 05627-14
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC6

Quant Time: Dec 15 06:29:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

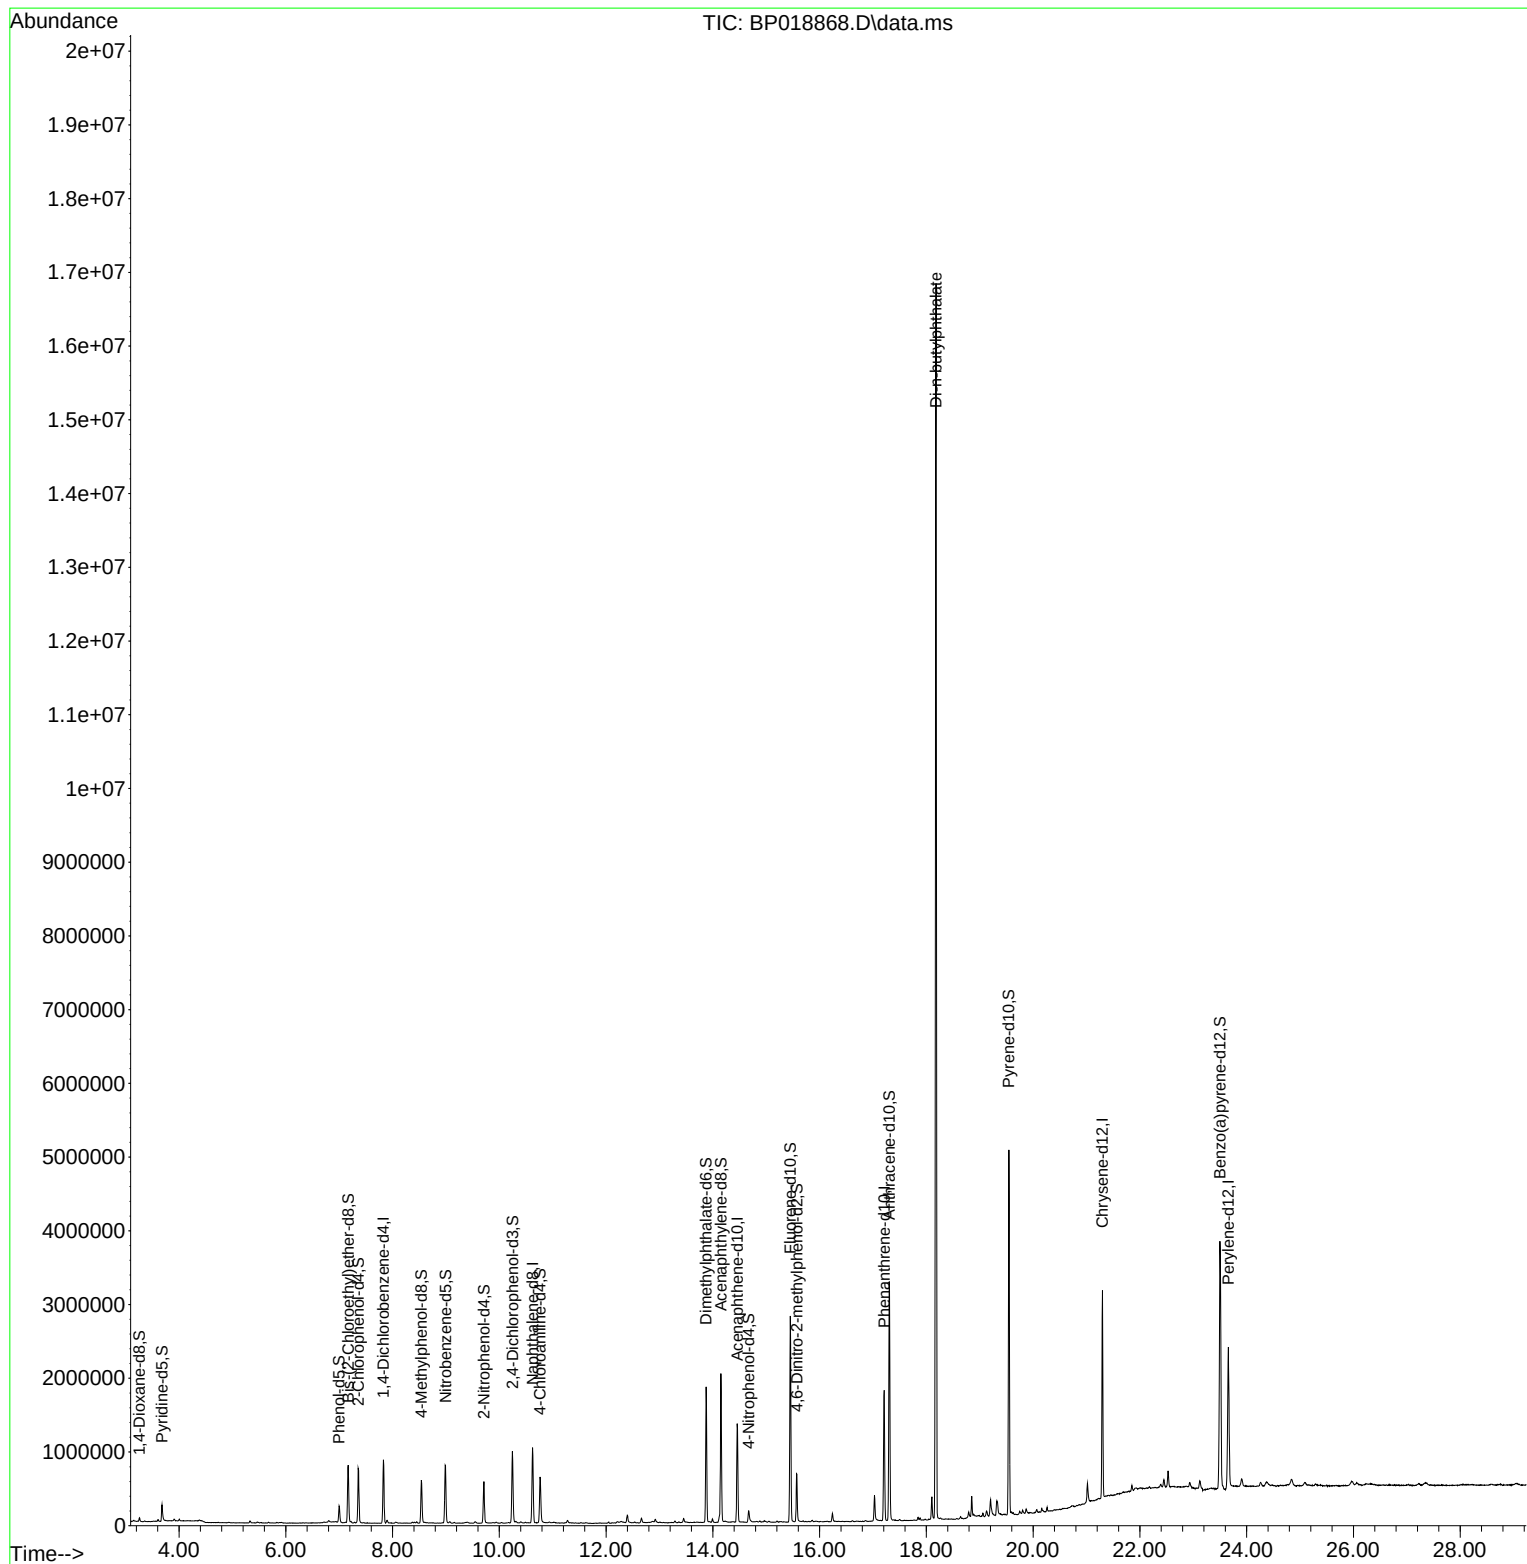

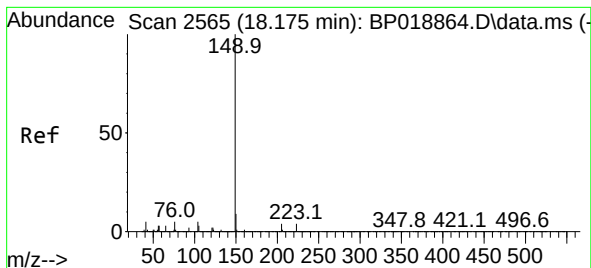

#78

Di-n-butylphthalate

Concen: 188.149 ng/ul

RT: 18.181 min Scan# 2

Delta R.T. 0.000 min

Lab File: BP018868.D


Acq: 15 Dec 2023 06:00

Instrument :

BNA_P

ClientSampleId :

DCLC6

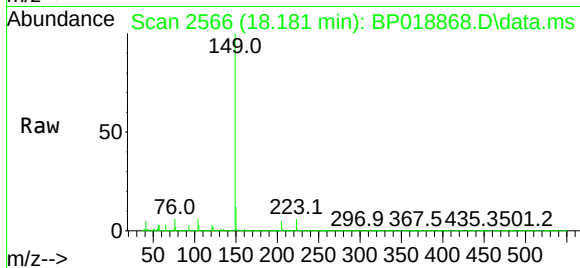

Tgt Ion:149 Resp:12993504

Ion Ratio Lower Upper

149 100

150 11.9 7.4 11.2#

104 6.2 3.9 5.9#

