

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018869.D
 Acq On : 15 Dec 2023 06:34
 Operator : MA/JU
 Sample : 05627-15
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC7

Quant Time: Dec 15 07:01:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	233001	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	826563	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	459556	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	959360	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1040863	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1254835	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	28646	4.190	ng/uL	0.00
4) Pyridine-d5	3.681	84	161310	8.808	ng/ul	0.00
7) Phenol-d5	6.999	99	150578	6.440	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.164	67	368366	26.580	ng/ul	0.00
11) 2-Chlorophenol-d4	7.358	132	393714	21.579	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	251293	13.280	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	218896	29.755	ng/ul	0.00
24) 2-Nitrophenol-d4	9.711	143	219291	28.751	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	412044	26.420	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	407494	19.993	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1286787	31.373	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	1446287	32.023	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	40822	6.063	ng/ul	0.00
60) Fluorene-d10	15.451	176	1125949	32.704	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	147164	25.583	ng/ul	0.00
73) Anthracene-d10	17.304	188	1844808	36.578	ng/ul	0.00
81) Pyrene-d10	19.545	212	2331642	28.778	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	2512427	34.339	ng/ul	-0.01
Target Compounds						
78) Di-n-butylphthalate	18.175	149	10153549	164.737	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018869.D
Acq On : 15 Dec 2023 06:34
Operator : MA/JU
Sample : 05627-15
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC7


Quant Time: Dec 15 07:01:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

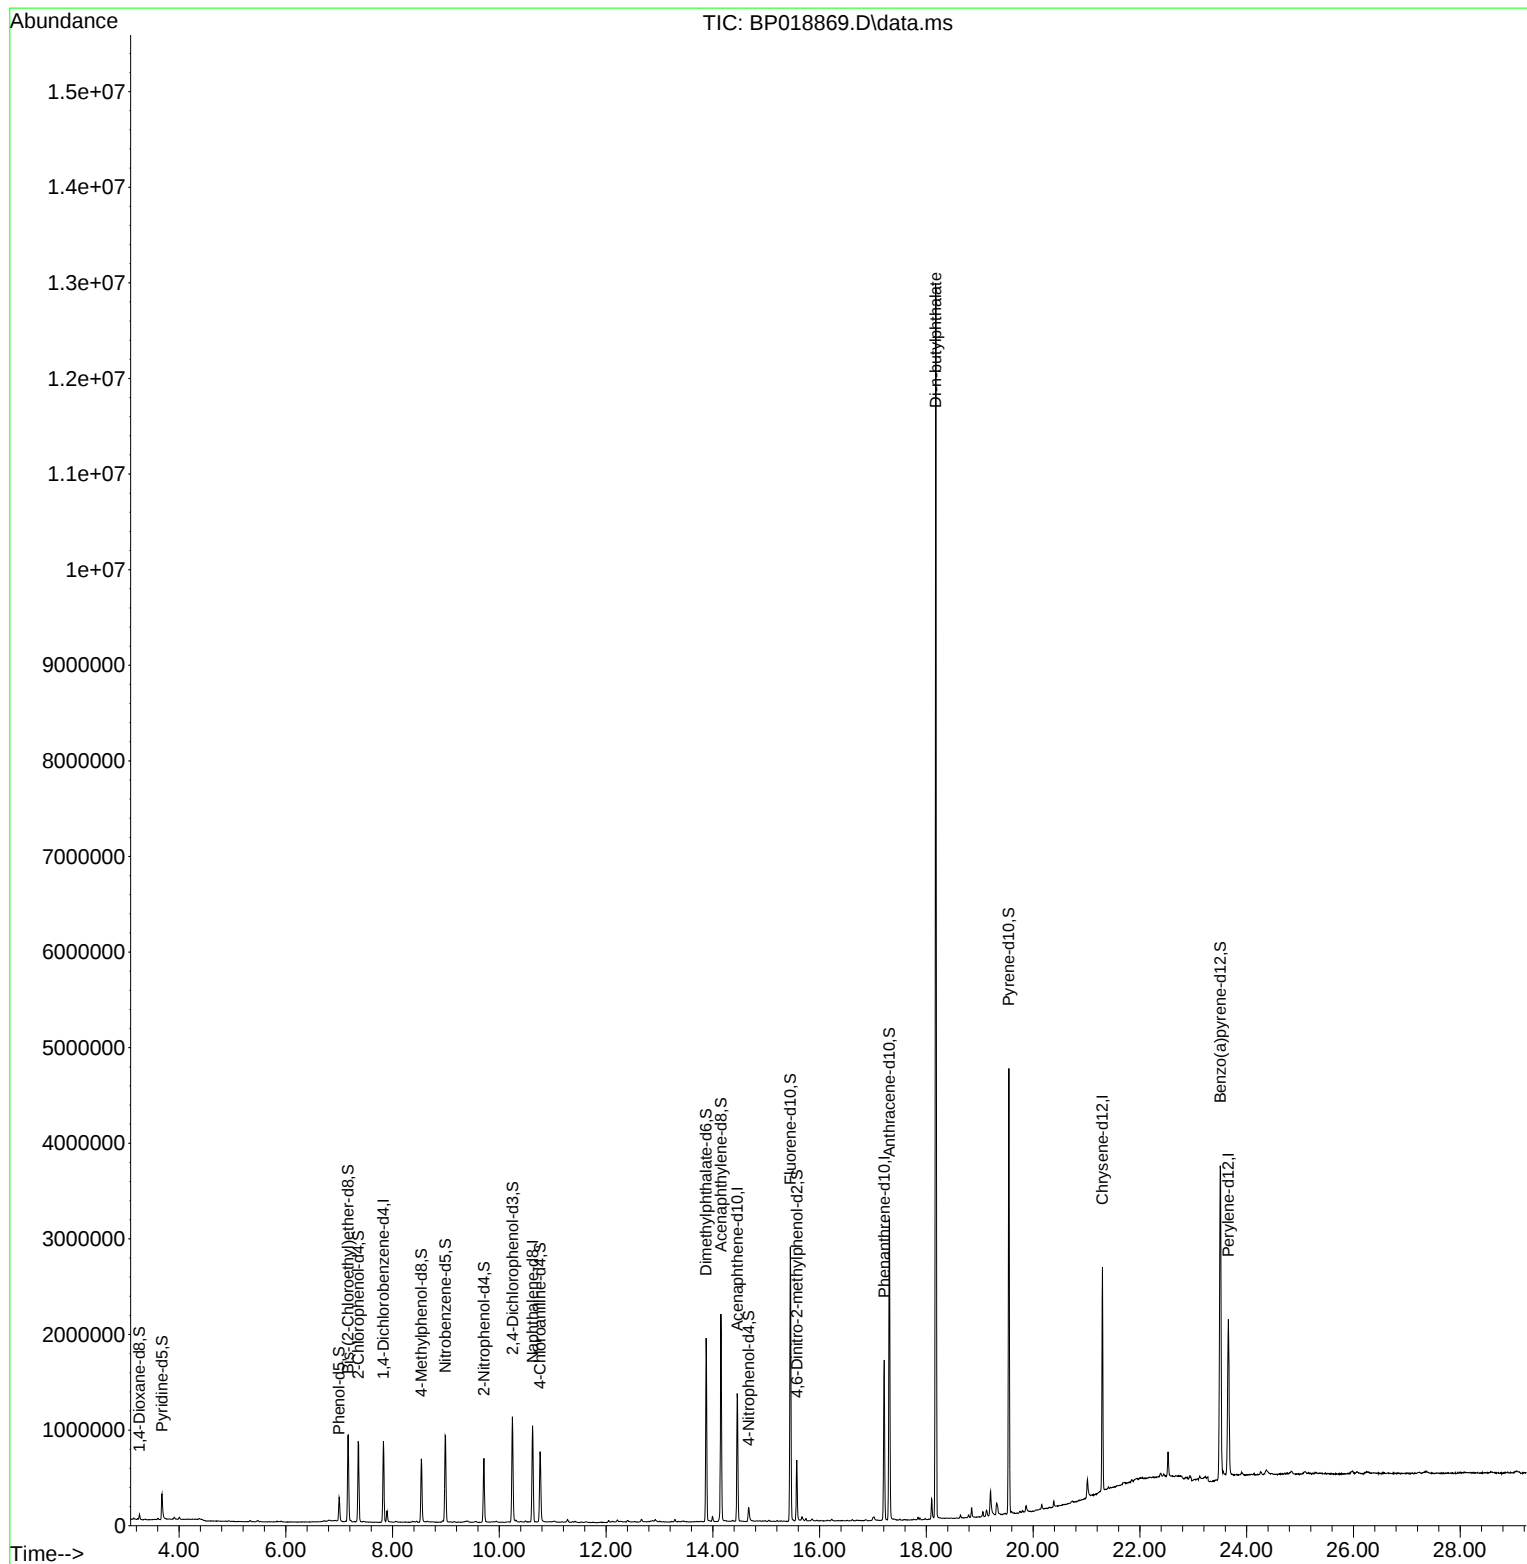

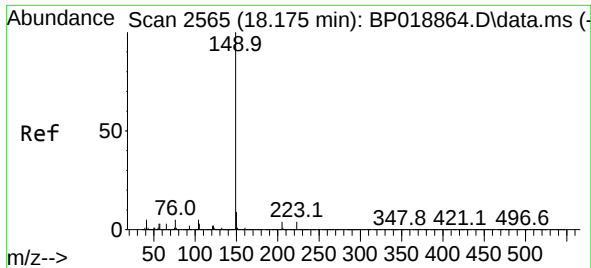

#78
Di-n-butylphthalate
Concen: 164.737 ng/ul
RT: 18.175 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP018869.D
Acq: 15 Dec 2023 06:34

Instrument :
BNA_P
ClientSampleId :
DCLC7

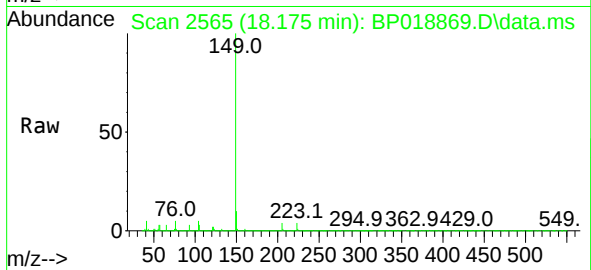

Tgt Ion:149 Resp:10153549
Ion Ratio Lower Upper
149 100
150 9.9 7.4 11.2
104 5.2 3.9 5.9

