

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018871.D
 Acq On : 15 Dec 2023 07:41
 Operator : MA/JU
 Sample : 05627-17
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC9

Quant Time: Dec 15 08:10:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	216314	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	767445	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	427577	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	883747	20.000	ng/ul	-0.01
79) Chrysene-d12	21.298	240	1091813	20.000	ng/ul	0.00
88) Perylene-d12	23.657	264	1308184	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	26707	4.207	ng/uL	0.00
4) Pyridine-d5	3.681	84	107470	6.321	ng/ul	0.00
7) Phenol-d5	6.999	99	155031	7.142	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	393036	30.548	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	425067	25.095	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	236175	13.444	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	210654	30.840	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	240863	34.012	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	443334	30.616	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	437937	23.142	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1398764	36.654	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	1554715	36.998	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	44181	7.053	ng/ul	0.00
60) Fluorene-d10	15.451	176	1232736	38.484	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	171359	32.338	ng/ul	0.00
73) Anthracene-d10	17.304	188	2044794	44.012	ng/ul	0.00
81) Pyrene-d10	19.545	212	2698953	31.757	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	3098467	40.622	ng/ul	0.00


Target Compounds					Qvalue
78) Di-n-butylphthalate	18.175	149	7315284	128.842 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018871.D
Acq On : 15 Dec 2023 07:41
Operator : MA/JU
Sample : 05627-17
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC9


Quant Time: Dec 15 08:10:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

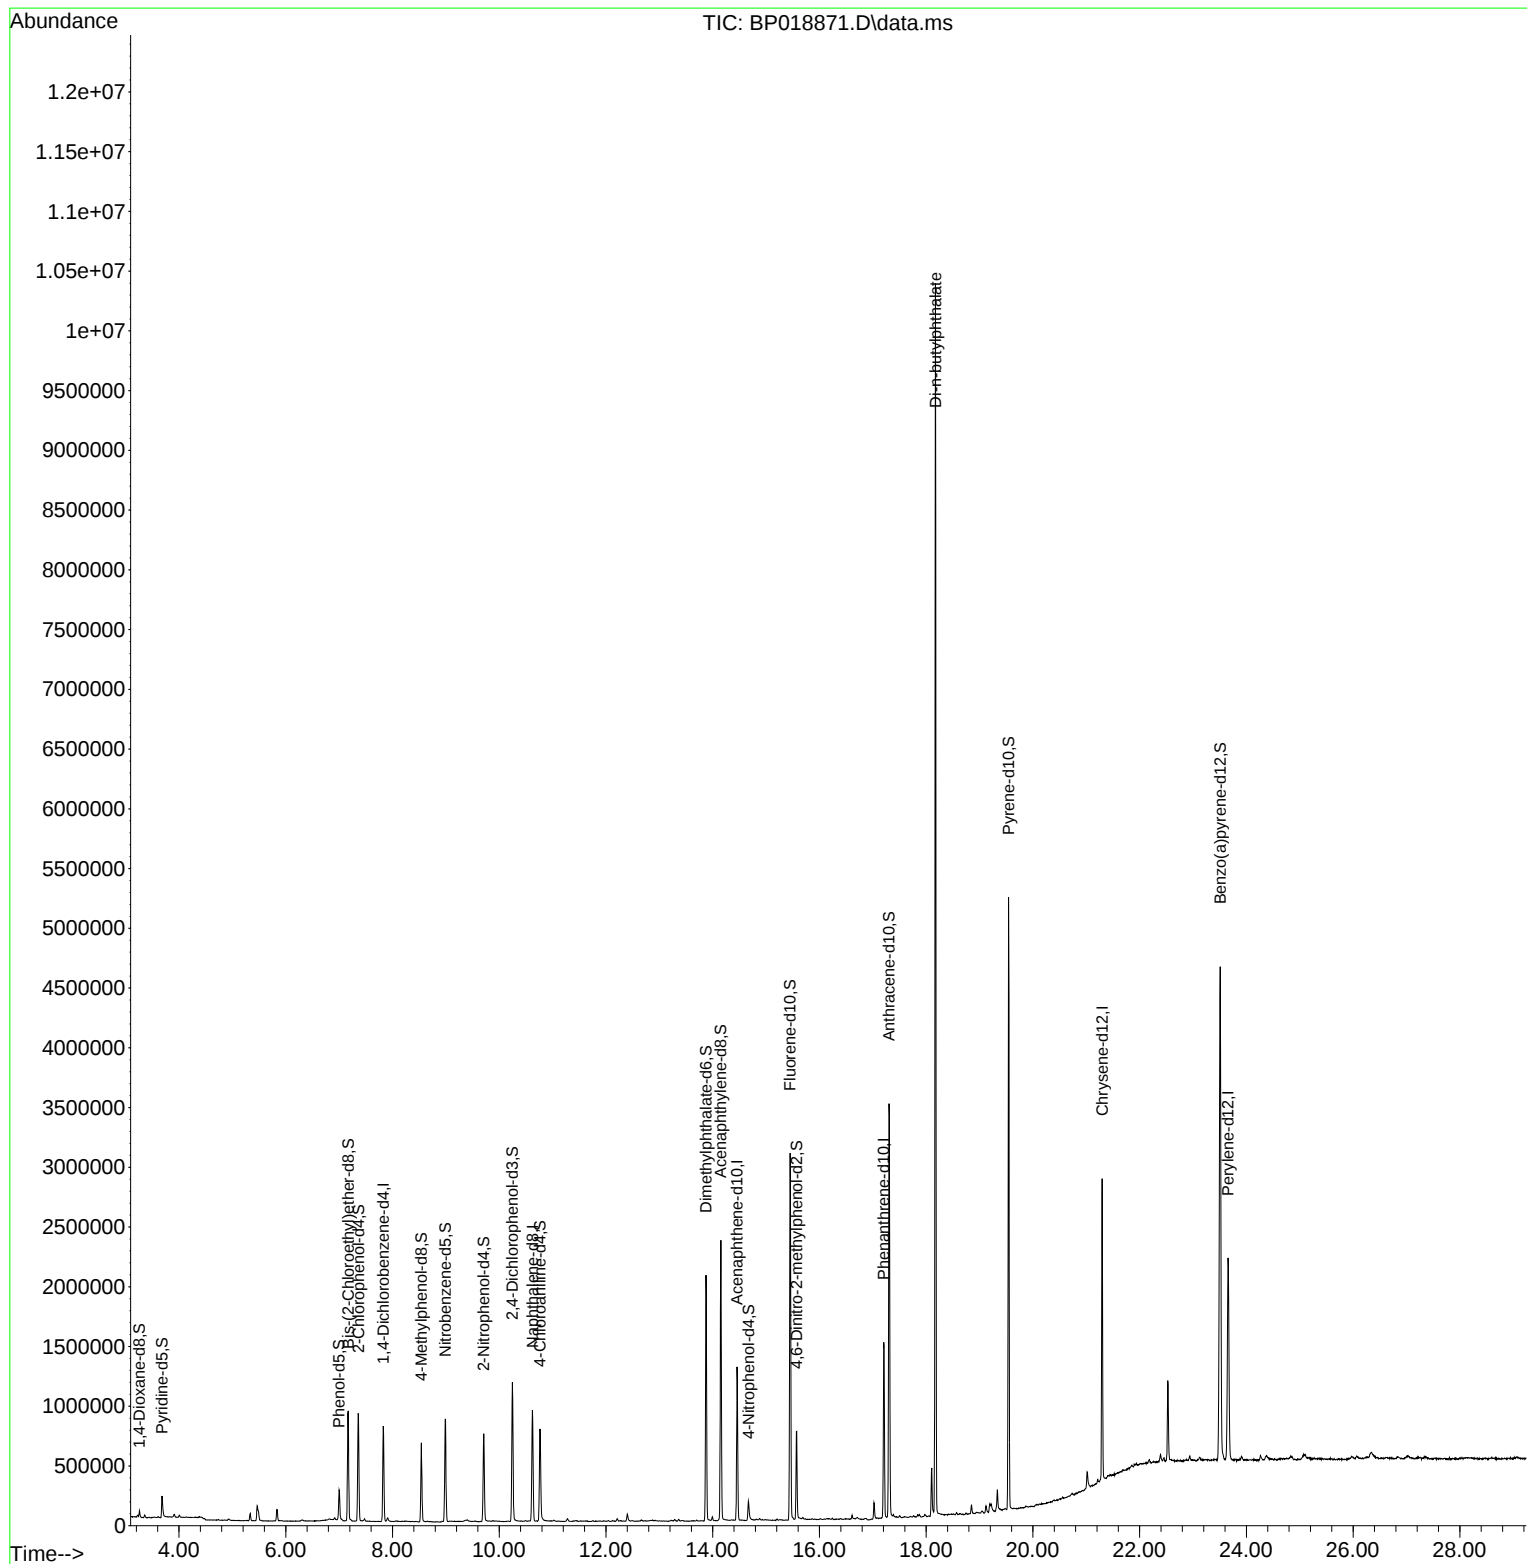

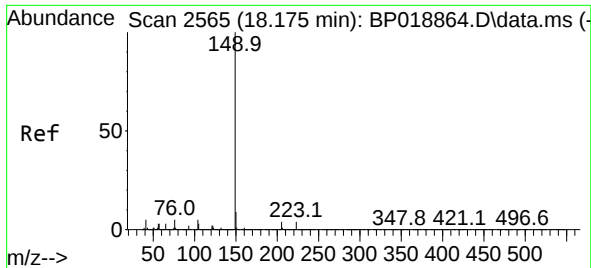

#78
 Di-n-butylphthalate
 Concen: 128.842 ng/ul
 RT: 18.175 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP018871.D
 Acq: 15 Dec 2023 07:41

Instrument :
 BNA_P
 ClientSampleId :
 DCLC9

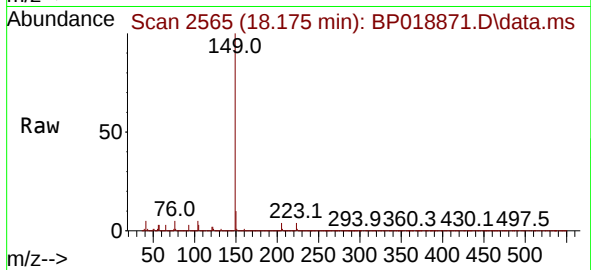

Tgt Ion:149 Resp: 7315284
 Ion Ratio Lower Upper
 149 100
 150 9.6 7.4 11.2
 104 5.2 3.9 5.9

