

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018876.D
 Acq On : 15 Dec 2023 11:29
 Operator : MA/JU
 Sample : 05627-13
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC5

Quant Time: Dec 15 12:11:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	215398	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.616	136	765157	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.457	164	420998	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	930105	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	1053720	20.000	ng/u1	0.00
88) Perylene-d12	23.663	264	1233140	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	25828	4.086	ng/uL	0.00
4) Pyridine-d5	3.676	84	154616	9.132	ng/u1	0.00
7) Phenol-d5	6.993	99	79367	3.672	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.158	67	318768	24.881	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.352	132	267786	15.876	ng/u1	-0.01
15) 4-Methylphenol-d8	8.534	113	19680	1.125	ng/u1	-0.01
21) Nitrobenzene-d5	8.987	128	185526	27.243	ng/u1	0.00
24) 2-Nitrophenol-d4	9.705	143	185012	26.204	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.240	165	258315	17.892	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.769	131	8610	0.456	ng/u1	0.00
46) Dimethylphthalate-d6	13.875	166	1156068	30.767	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	1132584	27.374	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	40000	6.485	ng/u1	0.00
60) Fluorene-d10	15.451	176	1022795	32.429	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	150140	26.922	ng/u1	0.00
73) Anthracene-d10	17.304	188	1271785	26.009	ng/u1	0.00
81) Pyrene-d10	19.545	212	1750943	21.347	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.510	264	2267811	31.541	ng/u1	0.00
Target Compounds						
78) Di-n-butylphthalate	18.175	149	3443298	57.623	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018876.D
Acq On : 15 Dec 2023 11:29
Operator : MA/JU
Sample : 05627-13
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC5


Quant Time: Dec 15 12:11:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

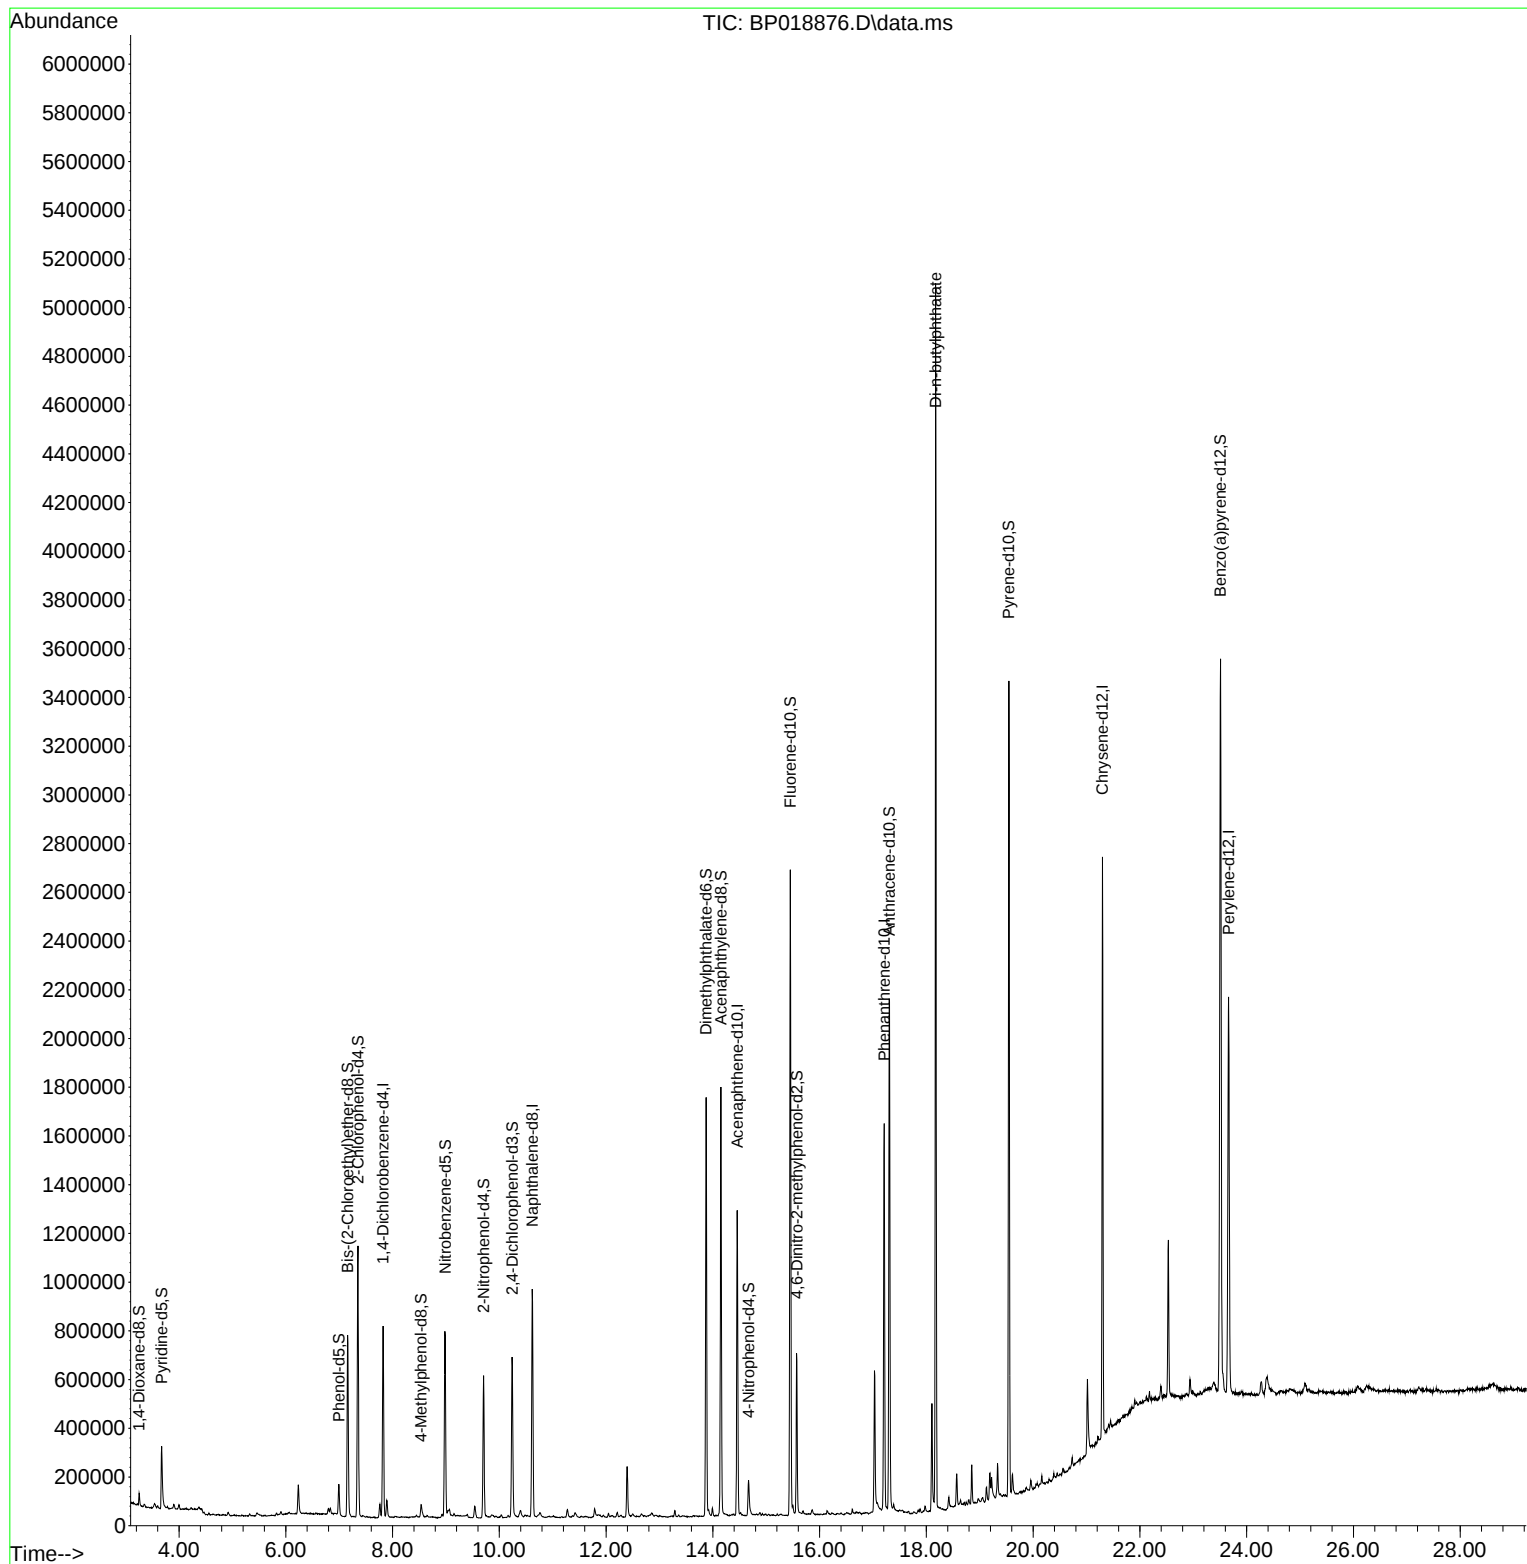

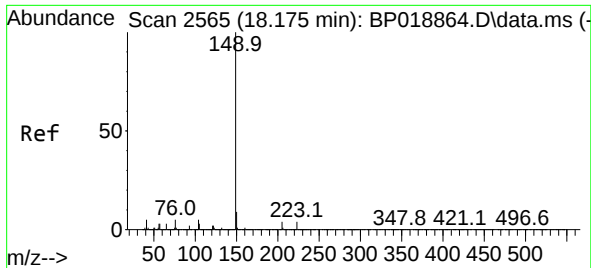

#78
 Di-n-butylphthalate
 Concen: 57.623 ng/ul
 RT: 18.175 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP018876.D
 Acq: 15 Dec 2023 11:29

Instrument :
 BNA_P
 ClientSampleId :
 DCLC5

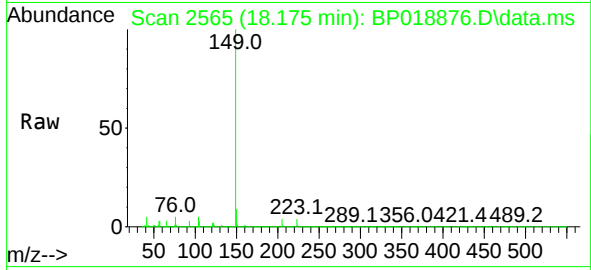

Tgt Ion:149 Resp: 3443298
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.2
 104 5.3 3.9 5.9

