

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018812.D
 Acq On : 13 Dec 2023 19:14
 Operator : MA/JU
 Sample : PB157657BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	40	rVB	92604	132886	1.50%	0.177%
2	3.675	96	100	120	rBV	1095484	1588643	17.96%	2.117%
3	4.005	153	156	162	rVB	16992	21122	0.24%	0.028%
4	7.005	658	666	680	rBV	1187440	1840343	20.81%	2.453%
5	7.175	688	695	705	rVB	959208	1523223	17.22%	2.030%
6	7.364	720	727	740	rBV	1198979	1873520	21.18%	2.497%
7	7.834	799	807	818	rVB	1004156	1551178	17.54%	2.068%
8	8.546	920	928	940	rBV	1430531	2261142	25.57%	3.014%
9	8.999	997	1005	1017	rBV	1028443	1695862	19.18%	2.260%
10	9.716	1117	1127	1141	rBV	843759	1356635	15.34%	1.808%
11	10.252	1211	1218	1239	rBV	1364648	2252420	25.47%	3.002%
12	10.628	1275	1282	1289	rBV	1257607	2075411	23.47%	2.766%
13	10.681	1289	1291	1296	rVB	14947	18663	0.21%	0.025%
14	10.769	1298	1306	1320	rBV	1311093	2255084	25.50%	3.006%
15	12.216	1545	1552	1558	rBV	25531	45171	0.51%	0.060%
16	12.293	1558	1565	1570	rVB2	15412	24774	0.28%	0.033%
17	12.510	1597	1602	1609	rVB3	8033	13975	0.16%	0.019%
18	13.304	1733	1737	1742	rVB3	6119	9264	0.10%	0.012%
19	13.369	1742	1748	1752	rBV2	19519	31165	0.35%	0.042%
20	13.446	1755	1761	1766	rBV7	4368	9524	0.11%	0.013%
21	13.881	1828	1835	1845	rBV	2484786	3325021	37.60%	4.432%
22	14.157	1875	1882	1898	rBV	2665368	3986253	45.07%	5.313%
23	14.463	1927	1934	1941	rBV	1880017	2785011	31.49%	3.712%
24	14.528	1941	1945	1951	rVB	35418	54432	0.62%	0.073%
25	14.669	1962	1969	1993	rBV	1030597	1650566	18.66%	2.200%
26	14.863	1998	2002	2011	rVB	27370	53006	0.60%	0.071%
27	15.457	2095	2103	2109	rBV	3666659	5156291	58.30%	6.873%
28	15.510	2109	2112	2117	rVV	44842	65690	0.74%	0.088%
29	15.575	2117	2123	2136	rVV	1065423	1433590	16.21%	1.911%
30	15.692	2140	2143	2150	rVB3	17611	31586	0.36%	0.042%
31	17.034	2367	2371	2375	rVB2	7923	10914	0.12%	0.015%
32	17.210	2394	2401	2406	rBV	2508555	3529273	39.91%	4.704%
33	17.251	2406	2408	2412	rVV	120196	148717	1.68%	0.198%
34	17.310	2412	2418	2435	rVB	4113996	5846250	66.11%	7.792%
35	18.104	2547	2553	2561	rBV4	61018	117000	1.32%	0.156%
36	18.269	2579	2581	2585	rVB3	8922	11156	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018812.D
Acq On : 13 Dec 2023 19:14
Operator : MA/JU
Sample : PB157657BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.575	2629	2633	2637	rBV7	7046	11299	0.13%	0.015%
38	19.128	2722	2727	2732	rBV2	59369	82593	0.93%	0.110%
39	19.192	2734	2738	2741	rVV	59093	86211	0.97%	0.115%
40	19.222	2741	2743	2753	rVB	60520	79929	0.90%	0.107%
41	19.339	2759	2763	2768	rBV4	35731	54962	0.62%	0.073%
42	19.551	2792	2799	2810	rBV	5595743	7518308	85.01%	10.021%
43	21.298	3091	3096	3106	rBV	3571394	4510798	51.01%	6.012%
44	23.510	3464	3472	3488	rVB2	4504917	8843657	100.00%	11.787%
45	23.663	3491	3498	3511	rVB	2496597	5053293	57.14%	6.735%




Sum of corrected areas: 75025811

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018812.D
Acq On : 13 Dec 2023 19:14
Operator : MA/JU
Sample : PB157657BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

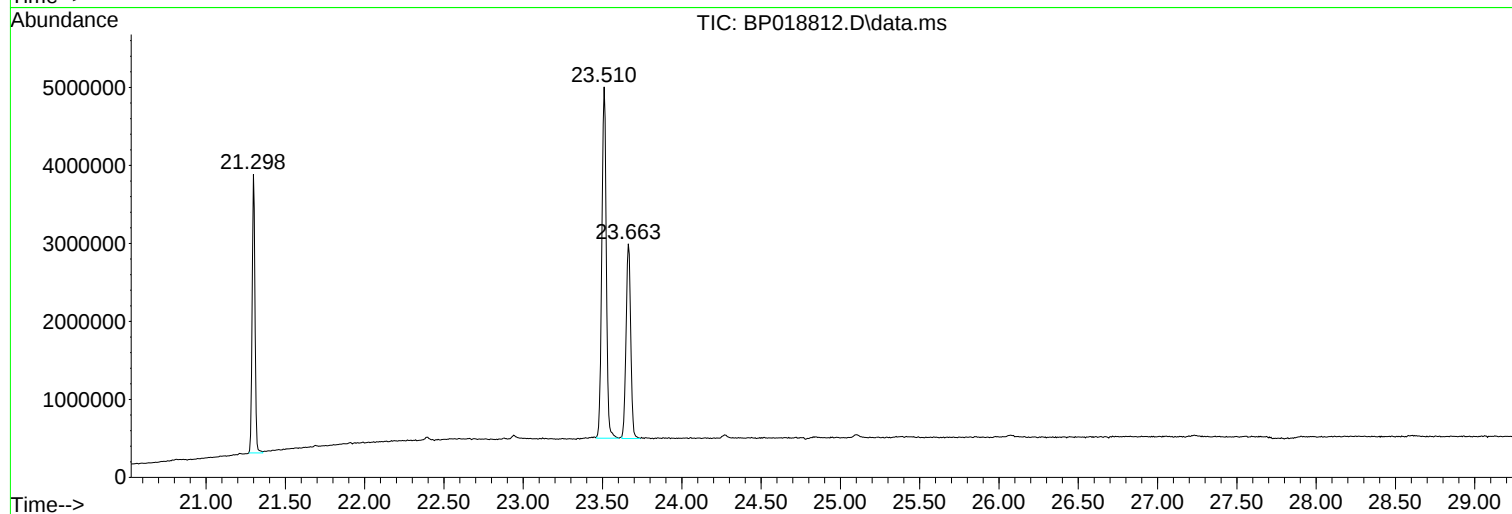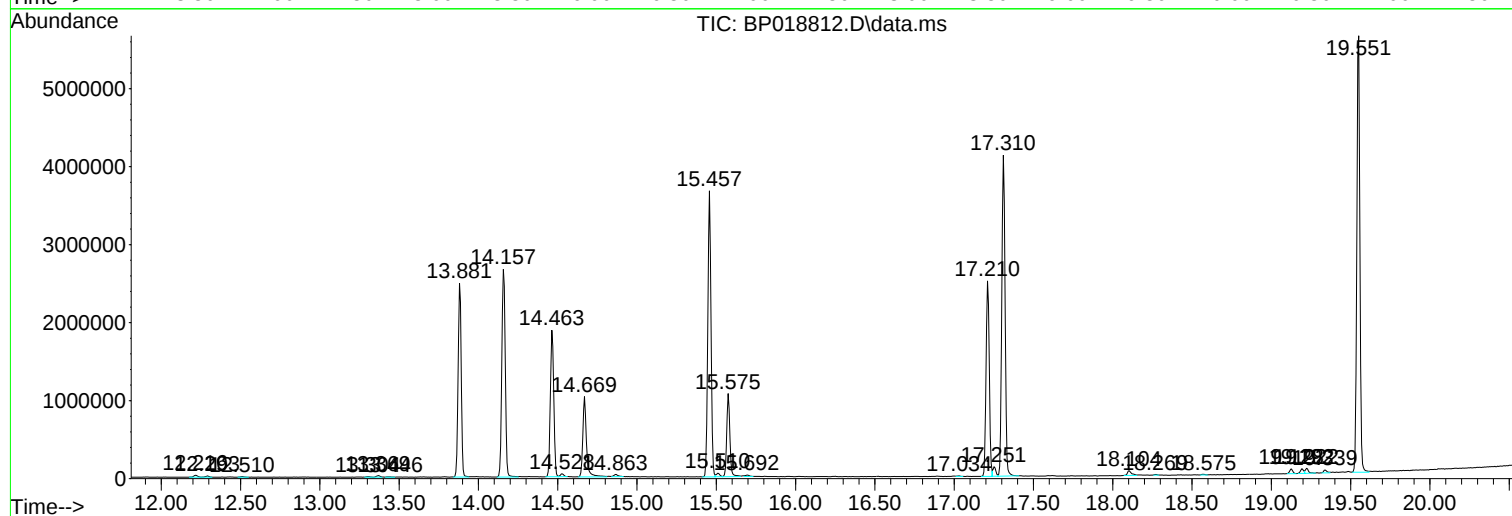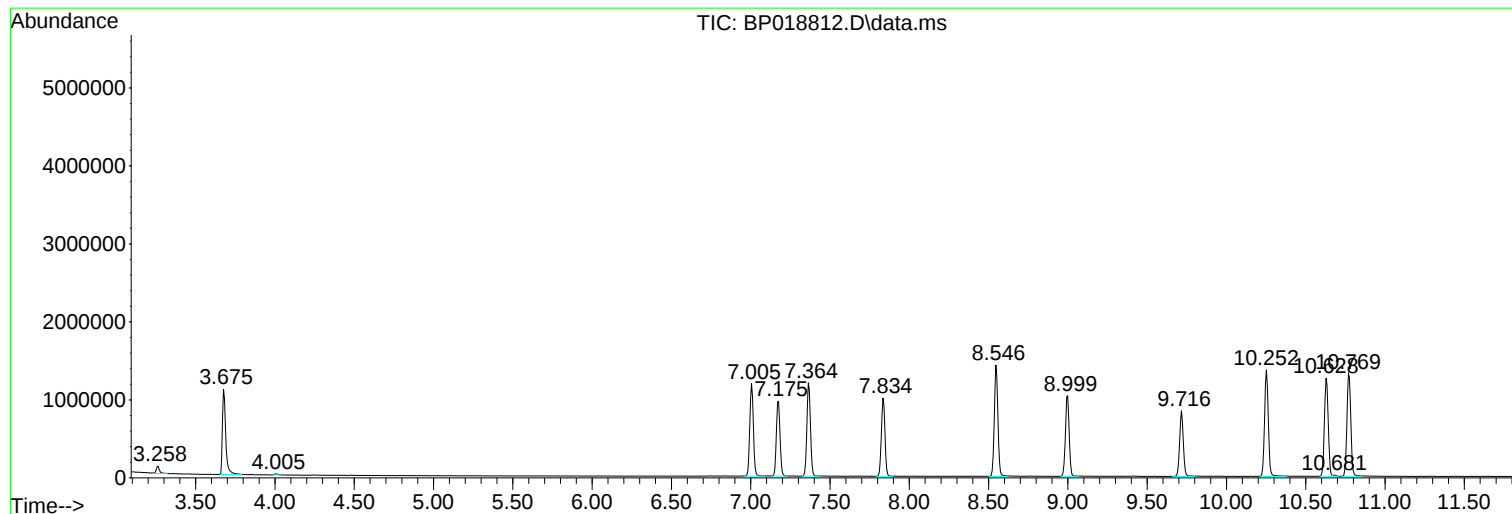

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018812.D
Acq On : 13 Dec 2023 19:14
Operator : MA/JU
Sample : PB157657BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018812.D
Acq On : 13 Dec 2023 19:14
Operator : MA/JU
Sample : PB157657BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc