

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018813.D
 Acq On : 13 Dec 2023 19:48
 Operator : MA/JU
 Sample : PB157680BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	37	rVB	78063	97758	1.60%	0.182%
2	3.675	96	100	115	rBV	859858	1218743	19.99%	2.266%
3	4.011	151	157	162	rVB	17207	26946	0.44%	0.050%
4	4.493	231	239	241	rBV4	7160	16573	0.27%	0.031%
5	5.546	411	418	423	rBV4	4714	11441	0.19%	0.021%
6	7.005	657	666	674	rBV	916163	1406121	23.06%	2.614%
7	7.169	688	694	704	rVB	755941	1174871	19.27%	2.184%
8	7.363	718	727	737	rBV	925385	1443283	23.67%	2.683%
9	7.834	800	807	817	rBV	851830	1305256	21.40%	2.427%
10	8.546	919	928	946	rBV	1073712	1697861	27.84%	3.157%
11	8.763	958	965	968	rBV9	2992	7060	0.12%	0.013%
12	8.993	996	1004	1014	rBV	790667	1281265	21.01%	2.382%
13	9.416	1072	1076	1083	rVB8	6224	14366	0.24%	0.027%
14	9.716	1117	1127	1136	rBV	592919	988426	16.21%	1.838%
15	10.251	1210	1218	1229	rBV	1009966	1667494	27.34%	3.100%
16	10.628	1275	1282	1290	rVB	1044798	1697539	27.84%	3.156%
17	10.769	1296	1306	1318	rBV	971549	1663916	27.29%	3.093%
18	12.216	1546	1552	1558	rBV2	19193	34735	0.57%	0.065%
19	12.422	1583	1587	1591	rBV7	3542	6717	0.11%	0.012%
20	13.369	1744	1748	1755	rVB2	19305	31574	0.52%	0.059%
21	13.434	1755	1759	1767	rVB10	3458	7013	0.12%	0.013%
22	13.881	1828	1835	1846	rBV	1729320	2380005	39.03%	4.425%
23	14.157	1874	1882	1893	rBV	1888139	2779997	45.59%	5.168%
24	14.463	1927	1934	1943	rBV	1496782	2150848	35.27%	3.999%
25	14.669	1963	1969	1989	rBV	666126	1123281	18.42%	2.088%
26	14.887	2002	2006	2010	rVB6	7177	10327	0.17%	0.019%
27	15.457	2094	2103	2115	rBV	2519698	3611285	59.22%	6.714%
28	15.575	2117	2123	2138	rVV	634108	893331	14.65%	1.661%
29	15.692	2140	2143	2147	rVB5	11647	15968	0.26%	0.030%
30	16.028	2195	2200	2203	rBV7	4986	7955	0.13%	0.015%
31	16.151	2218	2221	2230	rVB7	5400	10966	0.18%	0.020%
32	16.616	2297	2300	2305	rBV7	4625	7072	0.12%	0.013%
33	16.892	2343	2347	2351	rVB7	5449	7553	0.12%	0.014%
34	17.210	2394	2401	2408	rBV	1838431	2547084	41.77%	4.735%
35	17.310	2411	2418	2433	rVV	2924422	4113023	67.45%	7.647%
36	18.104	2547	2553	2562	rBV2	100438	173191	2.84%	0.322%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018813.D
Acq On : 13 Dec 2023 19:48
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.127	2722	2727	2732	rBV3	44139	63059	1.03%	0.117%
38	19.192	2734	2738	2742	rBV	42209	58433	0.96%	0.109%
39	19.339	2759	2763	2770	rBV	82132	117067	1.92%	0.218%
40	19.545	2793	2798	2805	rBV	3841059	5109816	83.79%	9.500%
41	21.298	3091	3096	3102	rBV	2567300	3199021	52.46%	5.947%
42	23.504	3464	3471	3479	rBV	3096976	6098082	100.00%	11.337%
43	23.663	3491	3498	3507	rVB	1718704	3511976	57.59%	6.529%




Sum of corrected areas: 53788298

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018813.D
Acq On : 13 Dec 2023 19:48
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

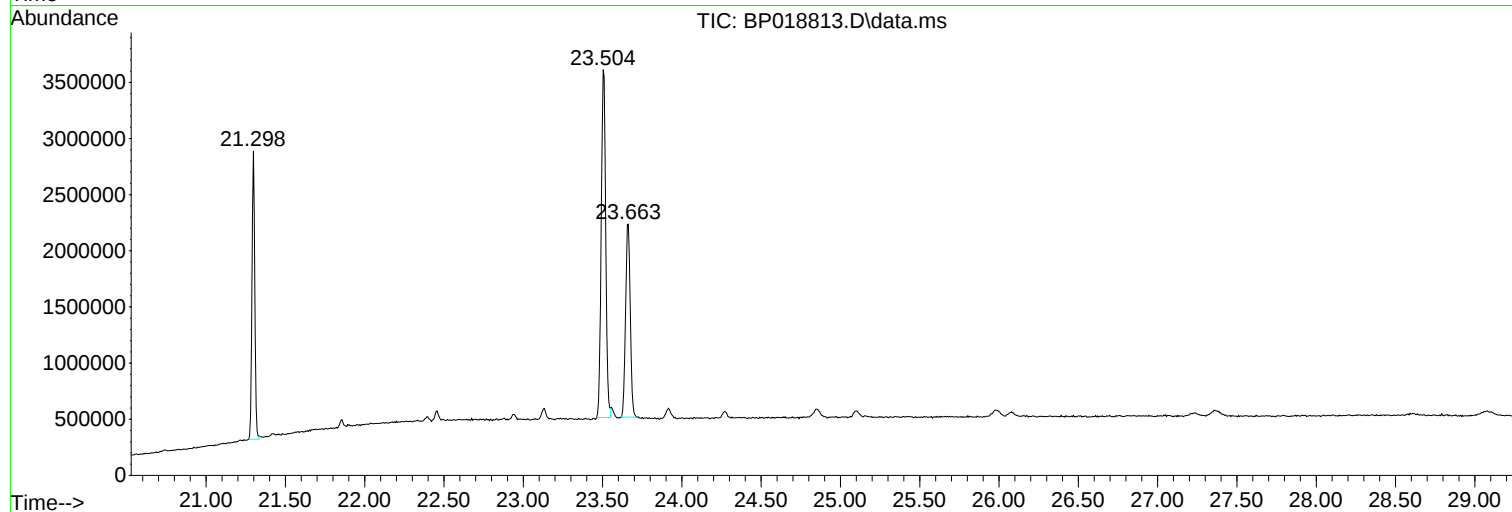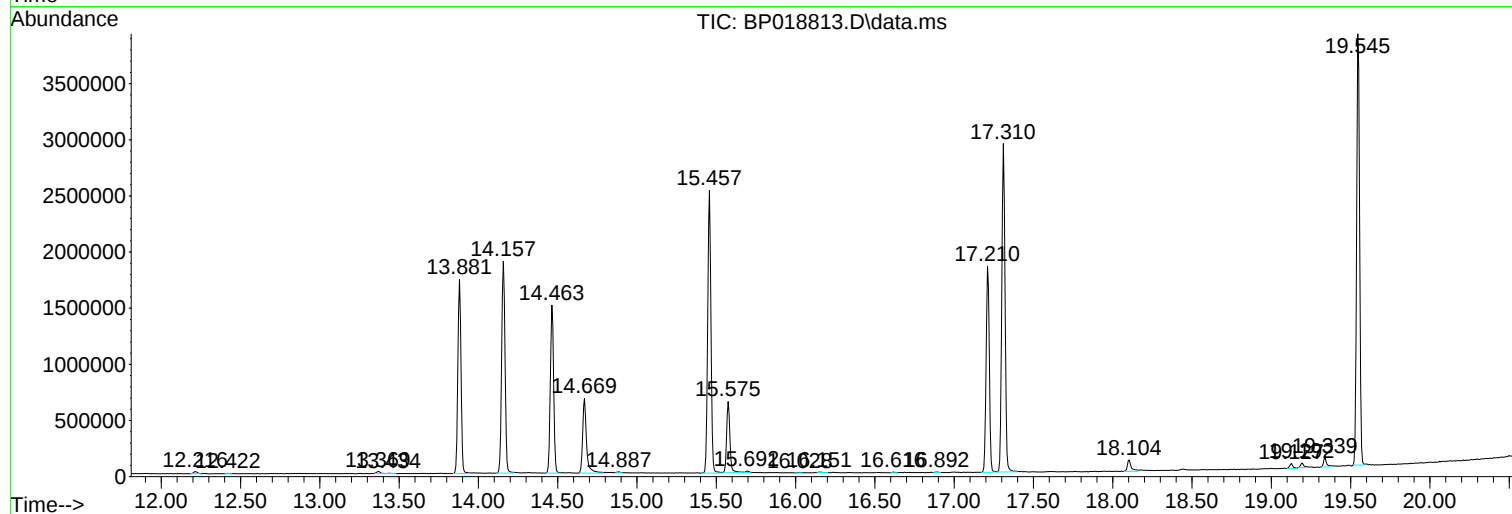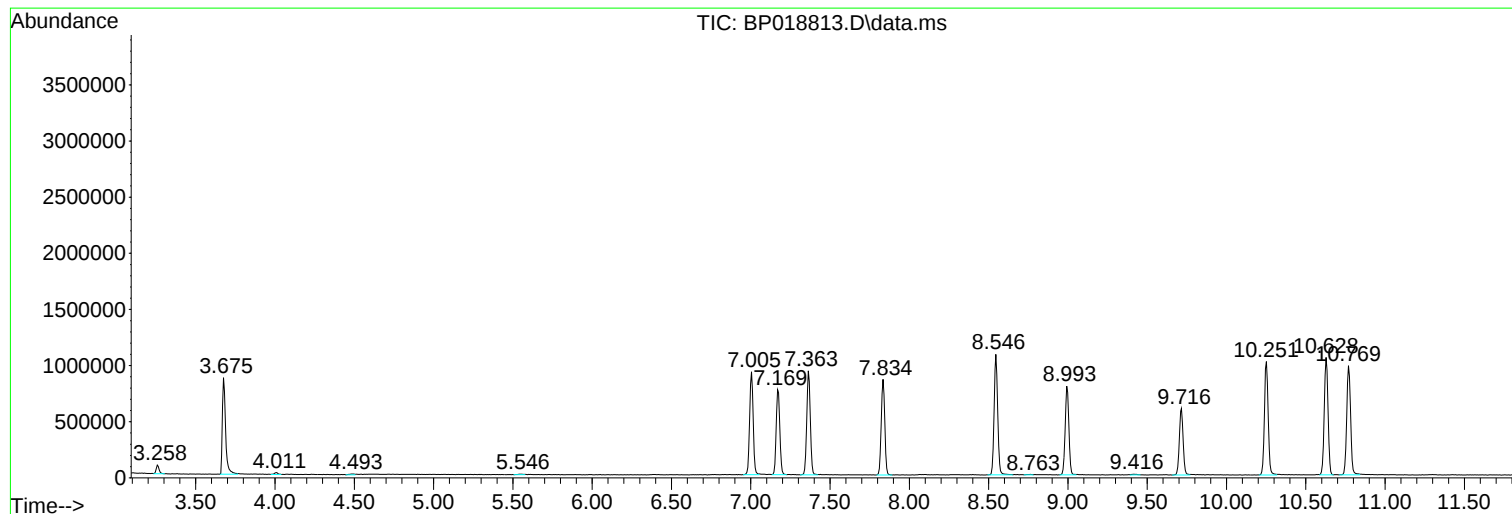

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018813.D
Acq On : 13 Dec 2023 19:48
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018813.D
Acq On : 13 Dec 2023 19:48
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------