

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018821.D
 Acq On : 14 Dec 2023 00:19
 Operator : MA/JU
 Sample : 05675-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	27	rBV	46335	69238	0.86%	0.110%
2	3.258	27	29	33	rVV	67250	82907	1.03%	0.132%
3	3.293	33	35	43	rVB	41422	49917	0.62%	0.079%
4	3.681	97	101	117	rBV	349089	522838	6.48%	0.831%
5	3.917	135	141	146	rVB	20679	35822	0.44%	0.057%
6	4.005	153	156	162	rVB	17946	23908	0.30%	0.038%
7	4.440	228	230	234	rVB2	8469	9432	0.12%	0.015%
8	4.540	240	247	256	rBV	343689	500365	6.21%	0.796%
9	4.928	308	313	319	rBV6	5056	11722	0.15%	0.019%
10	5.540	414	417	424	rVB8	6930	12352	0.15%	0.020%
11	7.005	659	666	676	rVB	224231	360079	4.47%	0.573%
12	7.169	688	694	705	rVB	966085	1499467	18.60%	2.384%
13	7.364	719	727	738	rBV	904146	1402539	17.39%	2.230%
14	7.463	740	744	753	rVB	5843	11234	0.14%	0.018%
15	7.834	799	807	816	rBV	1012779	1561887	19.37%	2.484%
16	8.546	921	928	936	rBV	649345	1016808	12.61%	1.617%
17	8.993	997	1004	1019	rBV	1037922	1656556	20.54%	2.634%
18	9.716	1118	1127	1141	rBV	759315	1240623	15.39%	1.973%
19	10.252	1210	1218	1228	rBV	1206728	1984284	24.61%	3.155%
20	10.628	1274	1282	1290	rBV	1208435	2017190	25.02%	3.208%
21	10.769	1298	1306	1320	rBV	1077879	1823258	22.61%	2.899%
22	11.381	1406	1410	1414	rBV6	6680	11761	0.15%	0.019%
23	11.428	1414	1418	1424	rVB9	5947	11166	0.14%	0.018%
24	12.046	1519	1523	1529	rBV8	4899	9163	0.11%	0.015%
25	12.216	1546	1552	1557	rBV	22563	36754	0.46%	0.058%
26	12.828	1652	1656	1659	rBV6	7099	9353	0.12%	0.015%
27	13.369	1744	1748	1754	rVB2	17079	26048	0.32%	0.041%
28	13.881	1828	1835	1845	rBV	2106682	3010035	37.33%	4.786%
29	13.969	1848	1850	1859	rVB10	4906	10206	0.13%	0.016%
30	14.157	1874	1882	1895	rBV	2532962	3752023	46.53%	5.966%
31	14.463	1927	1934	1942	rBV	1749120	2497225	30.97%	3.971%
32	14.669	1964	1969	1982	rBV	107859	224195	2.78%	0.357%
33	14.881	2000	2005	2012	rVB	10105	16617	0.21%	0.026%
34	15.457	2096	2103	2115	rBV	3350645	4810015	59.65%	7.649%
35	15.575	2117	2123	2139	rVV	736628	1052511	13.05%	1.674%
36	15.692	2139	2143	2150	rVB3	18212	33494	0.42%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018821.D
 Acq On : 14 Dec 2023 00:19
 Operator : MA/JU
 Sample : 05675-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.022	2195	2199	2204	rBV7	7334	13502	0.17%	0.021%
38	16.422	2262	2267	2270	rBV7	5145	9408	0.12%	0.015%
39	16.528	2278	2285	2289	rBV9	5020	12743	0.16%	0.020%
40	16.622	2297	2301	2305	rBV6	5640	8413	0.10%	0.013%
41	17.210	2394	2401	2411	rBV	2078198	2948167	36.56%	4.688%
42	17.310	2411	2418	2433	rVV	3715307	5205178	64.55%	8.277%
43	18.098	2548	2552	2560	rBV	103460	160519	1.99%	0.255%
44	19.122	2723	2726	2731	rVB	55036	67403	0.84%	0.107%
45	19.192	2734	2738	2741	rBV	50687	72938	0.90%	0.116%
46	19.333	2759	2762	2767	rBV2	75590	96269	1.19%	0.153%
47	19.545	2792	2798	2804	rBV	5108070	6632525	82.25%	10.547%
48	21.298	3091	3096	3103	rBV	3148579	3875237	48.06%	6.162%
49	23.510	3464	3472	3488	rVB2	4016761	8063436	100.00%	12.822%
50	23.663	3491	3498	3509	rVB	2155844	4317705	53.55%	6.866%




Sum of corrected areas: 62886435

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018821.D
Acq On : 14 Dec 2023 00:19
Operator : MA/JU
Sample : 05675-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

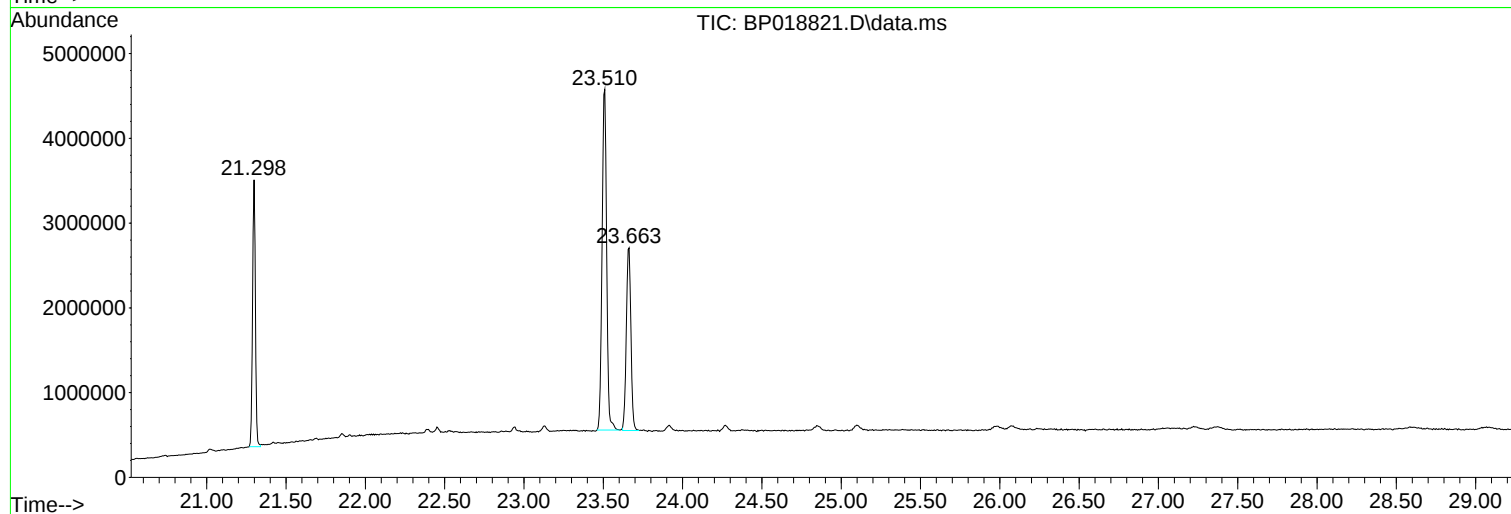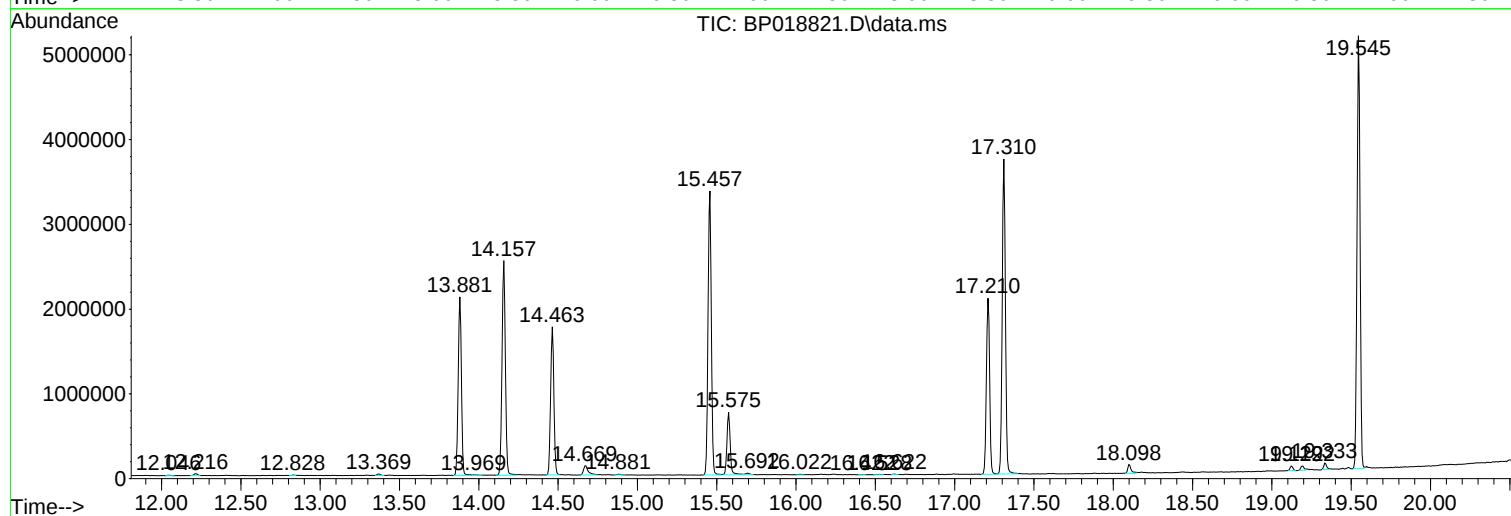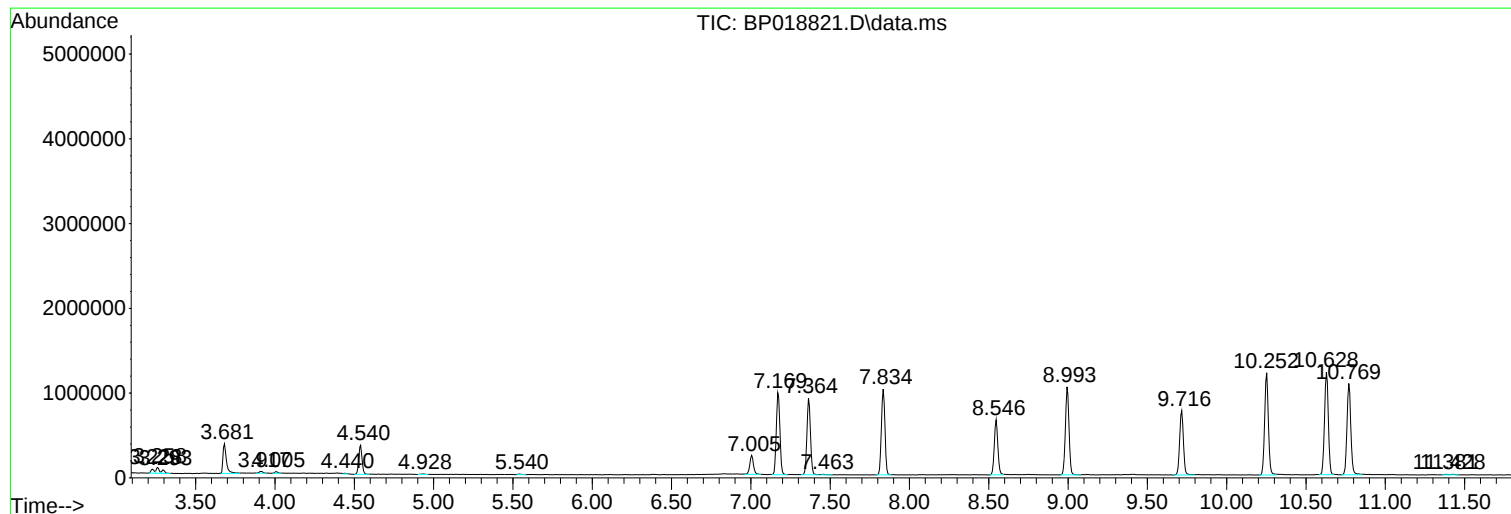

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018821.D
Acq On : 14 Dec 2023 00:19
Operator : MA/JU
Sample : 05675-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018821.D
Acq On : 14 Dec 2023 00:19
Operator : MA/JU
Sample : 05675-21
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc