

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018822.D
 Acq On : 14 Dec 2023 00:53
 Operator : MA/JU
 Sample : 05675-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	27	rBV	48587	69384	0.85%	0.106%
2	3.258	27	29	32	rVV	64273	72074	0.88%	0.110%
3	3.293	32	35	42	rVB	47011	65415	0.80%	0.100%
4	3.681	97	101	112	rBV	357846	540090	6.59%	0.827%
5	3.911	136	140	147	rBV2	23428	36971	0.45%	0.057%
6	4.005	153	156	161	rVB	16557	21520	0.26%	0.033%
7	4.540	241	247	256	rVB	358356	537818	6.56%	0.824%
8	4.934	309	314	320	rVB2	6614	10743	0.13%	0.016%
9	5.540	412	417	420	rBV6	6646	10397	0.13%	0.016%
10	7.005	660	666	674	rVB	247198	383705	4.68%	0.588%
11	7.169	688	694	704	rVB	1059860	1648812	20.11%	2.525%
12	7.363	719	727	738	rBV	986572	1532659	18.69%	2.347%
13	7.458	740	743	750	rVB9	7798	12773	0.16%	0.020%
14	7.834	798	807	816	rBV	1015989	1567272	19.12%	2.400%
15	8.546	920	928	938	rBV	717973	1125335	13.73%	1.723%
16	8.993	994	1004	1016	rBV	1119302	1826767	22.28%	2.797%
17	9.405	1072	1074	1079	rVB5	7489	12096	0.15%	0.019%
18	9.575	1097	1103	1110	rVB5	6886	13293	0.16%	0.020%
19	9.716	1117	1127	1135	rBV	841533	1354813	16.52%	2.075%
20	9.952	1162	1167	1171	rBV8	5516	10526	0.13%	0.016%
21	10.252	1209	1218	1235	rBV	1264425	2164156	26.40%	3.314%
22	10.628	1275	1282	1290	rBV	1264952	2042975	24.92%	3.128%
23	10.769	1299	1306	1319	rBV	1174981	1991836	24.29%	3.050%
24	11.381	1405	1410	1414	rBV4	15882	28419	0.35%	0.044%
25	11.422	1414	1417	1423	rVB7	6116	10005	0.12%	0.015%
26	12.051	1518	1524	1528	rBV4	12051	18371	0.22%	0.028%
27	12.216	1547	1552	1558	rBV	26006	42578	0.52%	0.065%
28	13.298	1730	1736	1740	rVB2	11415	17133	0.21%	0.026%
29	13.369	1743	1748	1753	rVB4	12868	21563	0.26%	0.033%
30	13.881	1828	1835	1849	rBV	2332038	3184310	38.84%	4.876%
31	14.157	1874	1882	1896	rBV	2754565	3971609	48.44%	6.082%
32	14.463	1927	1934	1941	rBV	1728140	2547339	31.07%	3.901%
33	14.669	1963	1969	1983	rBV	114004	247540	3.02%	0.379%
34	14.881	2000	2005	2010	rVB9	7778	15133	0.18%	0.023%
35	15.263	2065	2070	2073	rBV6	6611	11923	0.15%	0.018%
36	15.457	2096	2103	2116	rBV	3377532	5020678	61.24%	7.688%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018822.D
 Acq On : 14 Dec 2023 00:53
 Operator : MA/JU
 Sample : 05675-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.575	2117	2123	2137	rVV	807757	1115459	13.61%	1.708%
38	15.698	2140	2144	2153	rVB	18746	36735	0.45%	0.056%
39	16.028	2195	2200	2207	rBV	5049	10436	0.13%	0.016%
40	16.692	2310	2313	2318	rVB7	6313	9601	0.12%	0.015%
41	17.210	2394	2401	2411	rBV	2137110	2976372	36.30%	4.558%
42	17.310	2411	2418	2430	rVV	3841854	5374082	65.55%	8.229%
43	17.604	2463	2468	2479	rBV4	48892	113424	1.38%	0.174%
44	18.104	2549	2553	2562	rBV	124069	189009	2.31%	0.289%
45	19.122	2723	2726	2732	rVB2	56371	70120	0.86%	0.107%
46	19.192	2734	2738	2741	rBV	57848	77153	0.94%	0.118%
47	19.333	2759	2762	2767	rBV	62608	79779	0.97%	0.122%
48	19.545	2792	2798	2805	rBV	5055803	6758315	82.43%	10.349%
49	21.016	3046	3048	3055	rBV6	57147	94669	1.15%	0.145%
50	21.298	3091	3096	3102	rBV	3161887	3777751	46.08%	5.785%
51	23.504	3464	3471	3489	rVB2	4195496	8198862	100.00%	12.555%
52	23.657	3491	3497	3510	rVB	2077891	4234121	51.64%	6.484%




Sum of corrected areas: 65303919

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018822.D
Acq On : 14 Dec 2023 00:53
Operator : MA/JU
Sample : 05675-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

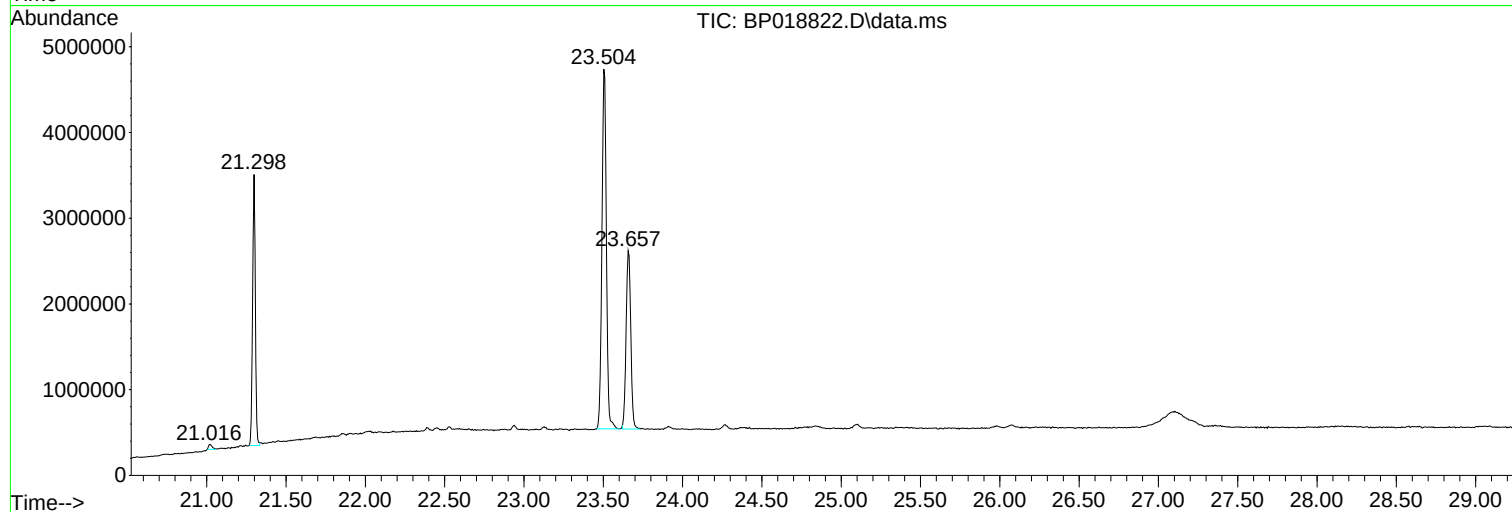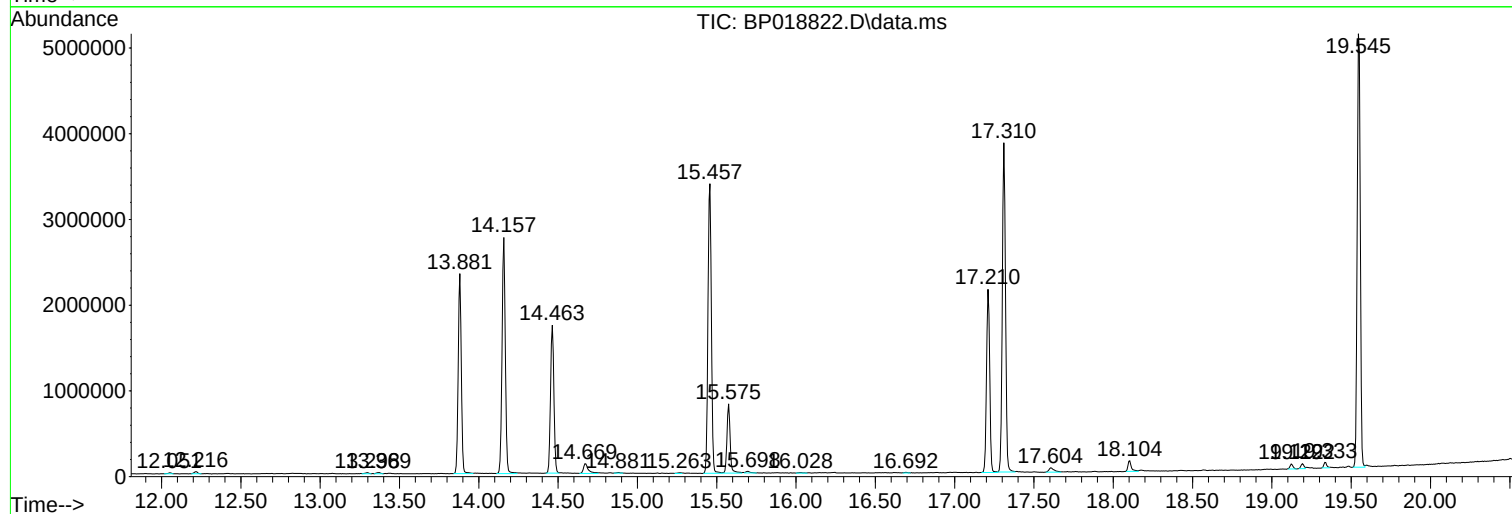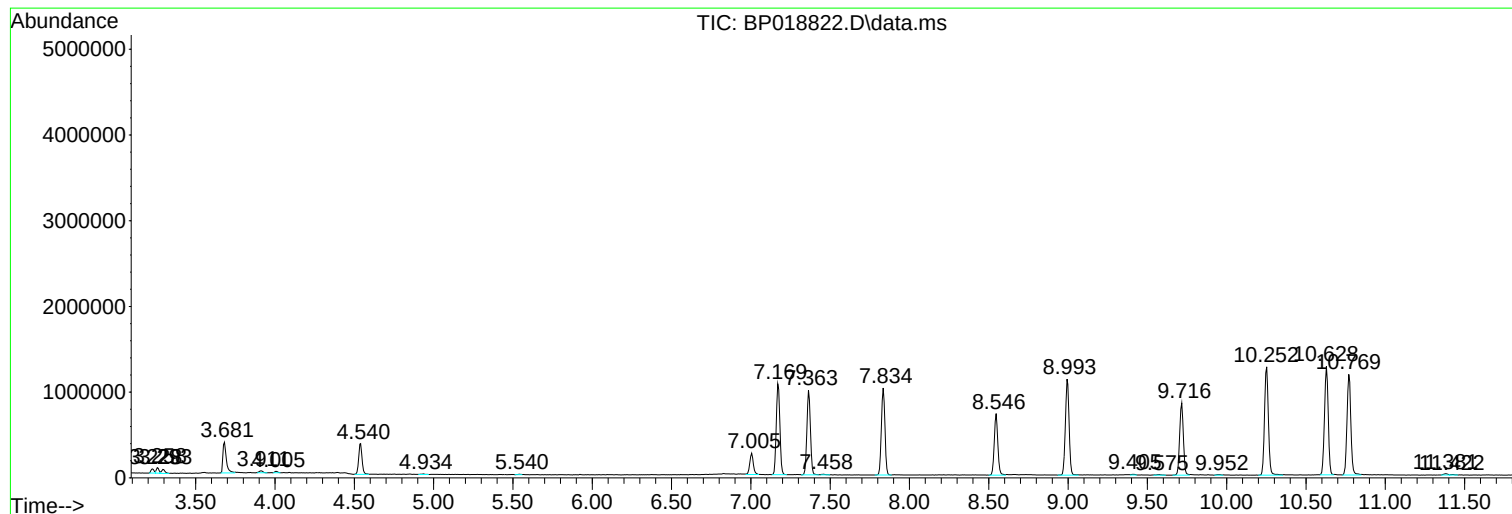

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018822.D
Acq On : 14 Dec 2023 00:53
Operator : MA/JU
Sample : 05675-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018822.D
Acq On : 14 Dec 2023 00:53
Operator : MA/JU
Sample : 05675-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
