

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018826.D
 Acq On : 14 Dec 2023 03:08
 Operator : MA/JU
 Sample : 05677-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	26	rBV	27417	38023	0.45%	0.062%
2	3.258	26	29	33	rVV	65844	82304	0.98%	0.133%
3	3.293	33	35	40	rVB	22306	25679	0.31%	0.042%
4	3.681	97	101	115	rBV	379130	601394	7.14%	0.975%
5	3.911	137	140	148	rVB2	21602	35023	0.42%	0.057%
6	4.011	153	157	164	rVB2	16656	23622	0.28%	0.038%
7	4.540	241	247	255	rVB	149677	230885	2.74%	0.374%
8	4.934	310	314	318	rBV5	7098	12344	0.15%	0.020%
9	6.828	633	636	639	rBV5	6371	8450	0.10%	0.014%
10	7.005	660	666	677	rVB	236127	388154	4.61%	0.629%
11	7.169	688	694	703	rVB	894787	1385134	16.45%	2.245%
12	7.363	719	727	738	rBV	883818	1356322	16.11%	2.199%
13	7.457	739	743	751	rVB	6238	13478	0.16%	0.022%
14	7.834	798	807	816	rBV	877448	1362347	16.18%	2.208%
15	8.546	921	928	937	rBV	644917	1019148	12.11%	1.652%
16	8.993	997	1004	1013	rBV	971653	1537735	18.27%	2.493%
17	9.410	1073	1075	1080	rVB6	7598	10558	0.13%	0.017%
18	9.716	1117	1127	1141	rBV	683331	1147215	13.63%	1.860%
19	10.251	1209	1218	1233	rBV	1115357	1889305	22.44%	3.063%
20	10.628	1275	1282	1294	rVB	1072075	1768980	21.01%	2.868%
21	10.769	1298	1306	1323	rBV	1052369	1762703	20.94%	2.858%
22	12.040	1516	1522	1528	rBV8	9446	24693	0.29%	0.040%
23	12.216	1545	1552	1556	rBV2	22613	36535	0.43%	0.059%
24	12.645	1620	1625	1629	rBV8	3834	8420	0.10%	0.014%
25	13.092	1696	1701	1705	rVB7	5265	10066	0.12%	0.016%
26	13.292	1731	1735	1743	rVB7	11880	17427	0.21%	0.028%
27	13.363	1743	1747	1754	rBV3	17084	28992	0.34%	0.047%
28	13.881	1828	1835	1847	rBV	2179760	2980830	35.41%	4.832%
29	14.157	1874	1882	1897	rBV	2470968	3563641	42.33%	5.777%
30	14.463	1926	1934	1942	rBV	1578567	2254468	26.78%	3.655%
31	14.563	1949	1951	1957	rVB7	5111	8588	0.10%	0.014%
32	14.669	1963	1969	1979	rBV	131452	255161	3.03%	0.414%
33	14.751	1979	1983	1991	rVB6	15237	32457	0.39%	0.053%
34	14.881	2001	2005	2012	rVB9	11154	20875	0.25%	0.034%
35	15.457	2096	2103	2116	rBV	3167833	4756628	56.50%	7.711%
36	15.575	2117	2123	2132	rVV	787836	1055276	12.54%	1.711%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018826.D
 Acq On : 14 Dec 2023 03:08
 Operator : MA/JU
 Sample : 05677-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.692	2140	2143	2150	rVB5	17966	27357	0.32%	0.044%
38	16.616	2297	2300	2304	rBV6	6130	10658	0.13%	0.017%
39	16.886	2343	2346	2351	rVB7	5865	9420	0.11%	0.015%
40	17.210	2395	2401	2408	rBV	1998094	2776849	32.99%	4.502%
41	17.310	2411	2418	2430	rBV	3901365	5401207	64.16%	8.756%
42	18.104	2548	2553	2558	rBV	149477	214153	2.54%	0.347%
43	19.122	2722	2726	2732	rVB3	59819	78590	0.93%	0.127%
44	19.192	2734	2738	2746	rBV	63094	104490	1.24%	0.169%
45	19.333	2758	2762	2767	rBV2	101871	132049	1.57%	0.214%
46	19.545	2792	2798	2804	rBV	5512183	7113929	84.50%	11.532%
47	21.298	3091	3096	3101	rBV	2982003	3604386	42.82%	5.843%
48	23.504	3464	3471	3486	rVB2	4164012	8418383	100.00%	13.647%
49	23.657	3491	3497	3509	rVB	2067707	4042529	48.02%	6.553%




Sum of corrected areas: 61686860

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018826.D
Acq On : 14 Dec 2023 03:08
Operator : MA/JU
Sample : 05677-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

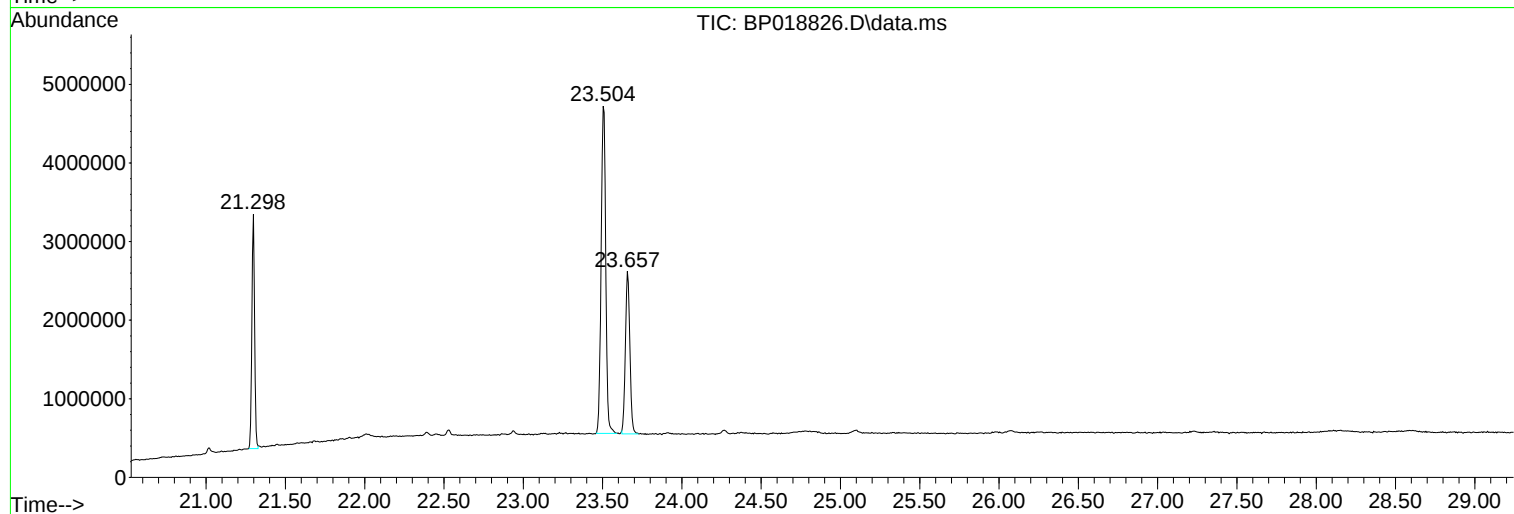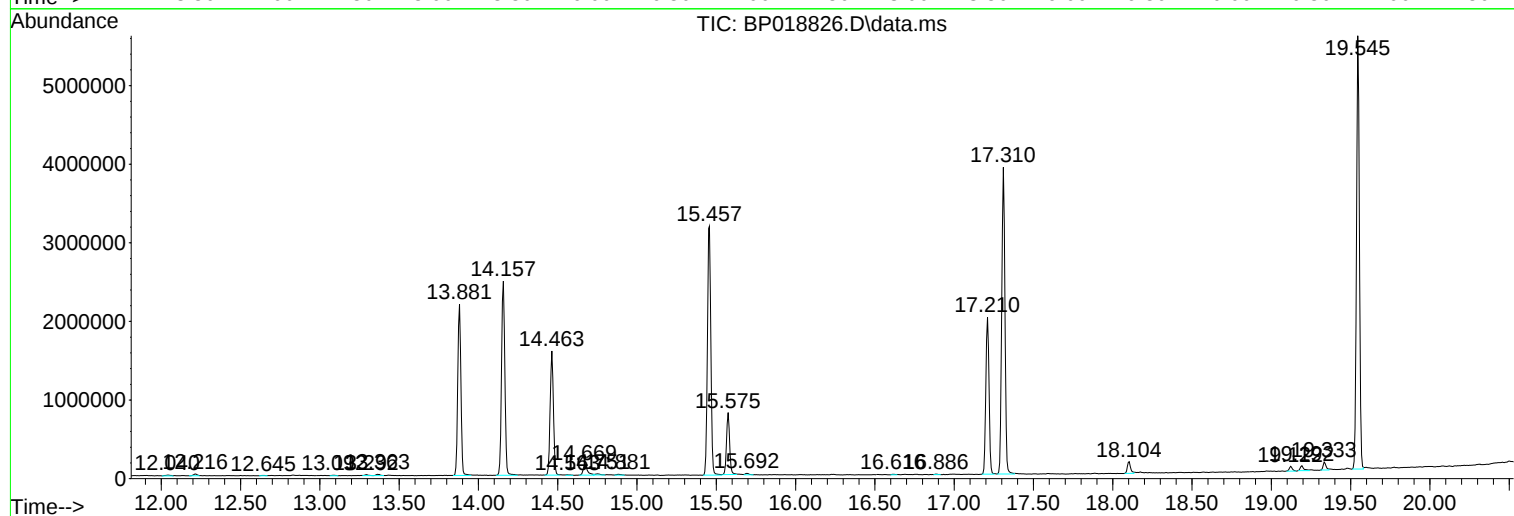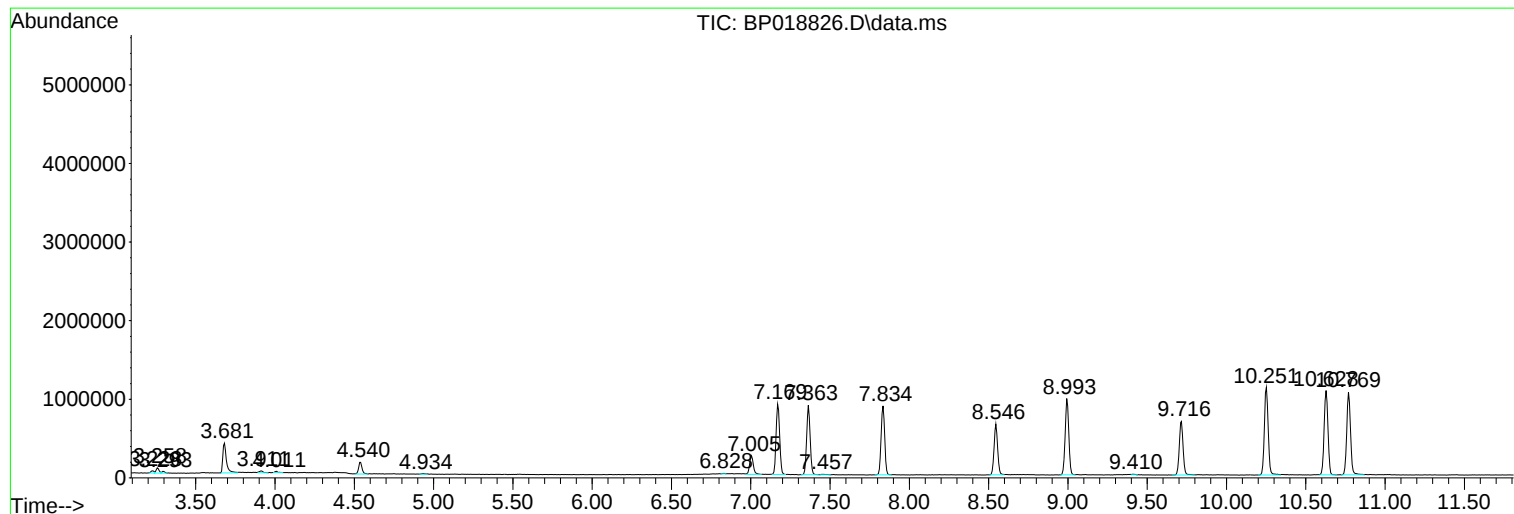

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018826.D
Acq On : 14 Dec 2023 03:08
Operator : MA/JU
Sample : 05677-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018826.D
Acq On : 14 Dec 2023 03:08
Operator : MA/JU
Sample : 05677-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc