

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018831.D
 Acq On : 14 Dec 2023 06:31
 Operator : MA/JU
 Sample : PB157722BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK722

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rBV	80511	99167	1.50%	0.176%
2	3.675	96	100	118	rBV	866189	1281913	19.42%	2.278%
3	4.005	153	156	164	rVB2	19001	28807	0.44%	0.051%
4	7.005	659	666	680	rVB	929592	1464172	22.18%	2.602%
5	7.169	688	694	703	rVB	796160	1214066	18.39%	2.157%
6	7.364	720	727	735	rBV	990745	1510116	22.87%	2.684%
7	7.834	799	807	815	rBV	920167	1442127	21.84%	2.563%
8	8.546	919	928	941	rBV	1111582	1756026	26.60%	3.121%
9	8.993	996	1004	1012	rBV	828081	1310395	19.85%	2.329%
10	9.716	1116	1127	1141	rBV	598910	1003825	15.21%	1.784%
11	10.252	1210	1218	1229	rBV	1008022	1727314	26.16%	3.070%
12	10.328	1229	1231	1238	rVB8	6019	11784	0.18%	0.021%
13	10.628	1274	1282	1291	rVB	1131432	1857497	28.14%	3.301%
14	10.769	1298	1306	1319	rBV	1005530	1699713	25.75%	3.020%
15	11.016	1345	1348	1355	rVB8	3774	7008	0.11%	0.012%
16	12.216	1545	1552	1557	rBV	19855	32361	0.49%	0.058%
17	12.828	1650	1656	1659	rBV7	7478	10982	0.17%	0.020%
18	13.369	1741	1748	1752	rBV4	20648	34456	0.52%	0.061%
19	13.434	1755	1759	1763	rVV7	4611	7654	0.12%	0.014%
20	13.881	1826	1835	1842	rBV	1662815	2336001	35.38%	4.151%
21	14.157	1875	1882	1893	rVV	1891457	2807764	42.53%	4.990%
22	14.463	1927	1934	1943	rBV	1548758	2294119	34.75%	4.077%
23	14.669	1962	1969	1992	rBV	604994	1115099	16.89%	1.982%
24	15.451	2096	2102	2116	rBV	2434347	3664360	55.50%	6.512%
25	15.575	2116	2123	2133	rVV	602184	829311	12.56%	1.474%
26	15.692	2139	2143	2149	rVB5	14605	21826	0.33%	0.039%
27	16.698	2310	2314	2316	rVB5	5661	7568	0.11%	0.013%
28	17.210	2394	2401	2408	rBV	1918462	2734103	41.41%	4.859%
29	17.310	2411	2418	2434	rVV	2969244	4184639	63.39%	7.436%
30	18.104	2549	2553	2558	rBV7	18095	30260	0.46%	0.054%
31	19.122	2722	2726	2731	rBV2	38369	53609	0.81%	0.095%
32	19.192	2734	2738	2747	rVV	35251	58200	0.88%	0.103%
33	19.545	2792	2798	2806	rBV	4131432	5436227	82.34%	9.661%
34	21.298	3091	3096	3102	rBV	2878474	3542482	53.66%	6.295%
35	23.504	3464	3471	3487	rVB2	3303917	6601865	100.00%	11.732%
36	23.657	3490	3497	3512	rVB	2092076	4055889	61.44%	7.208%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018831.D
Acq On : 14 Dec 2023 06:31
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 56272705

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018831.D
Acq On : 14 Dec 2023 06:31
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

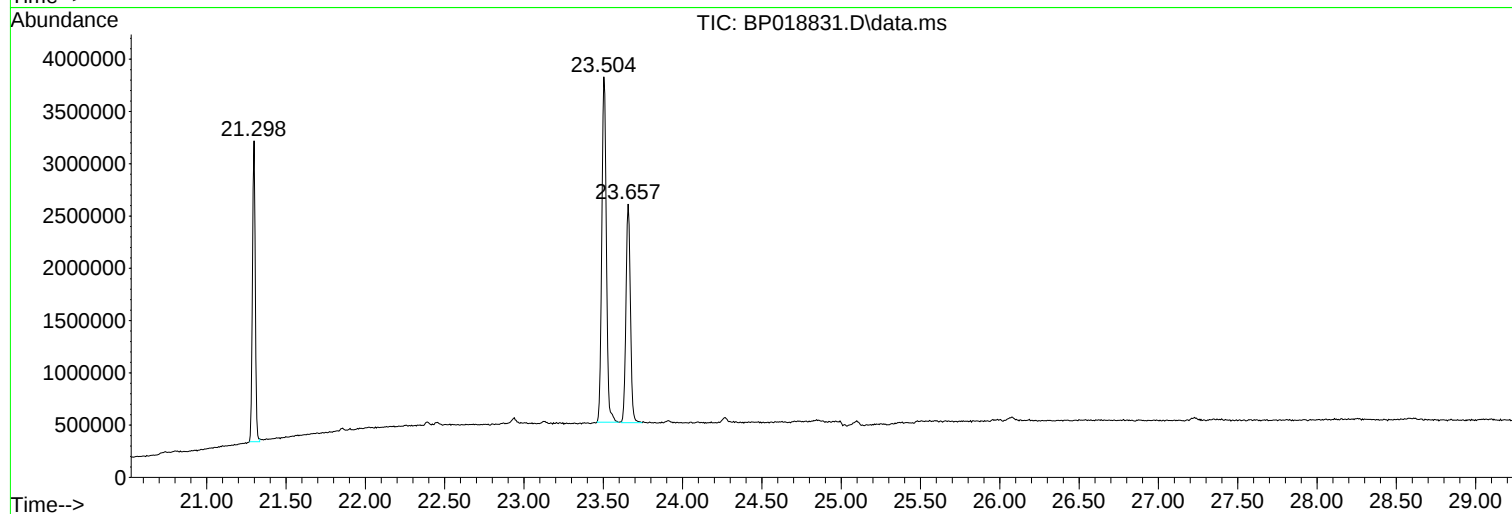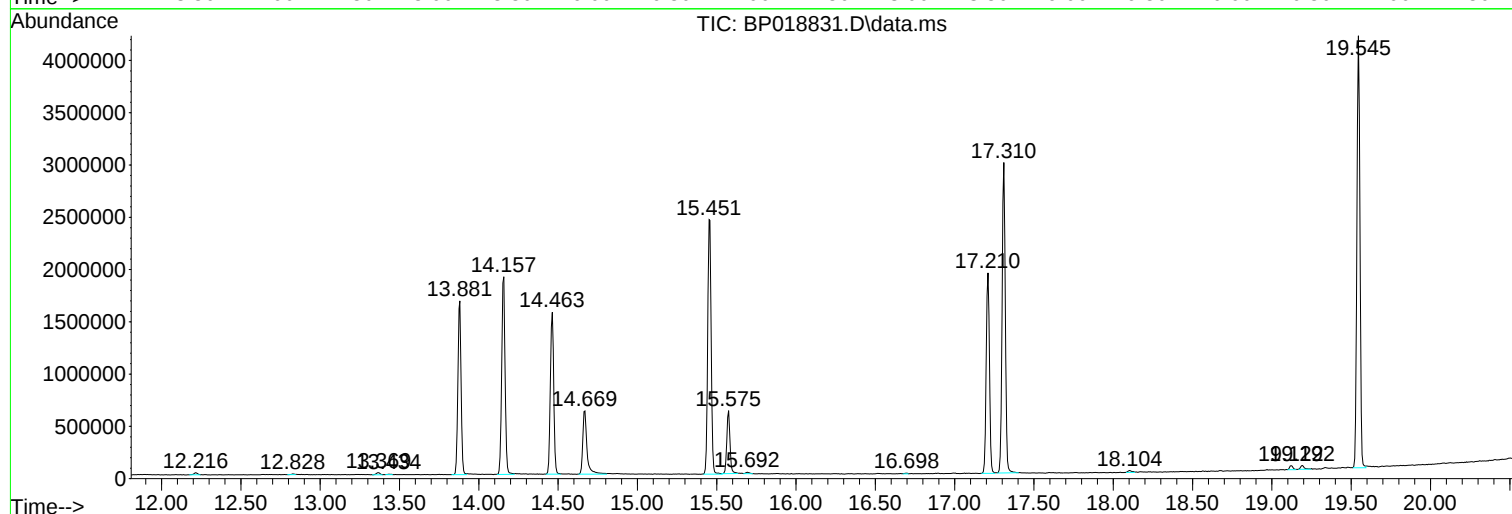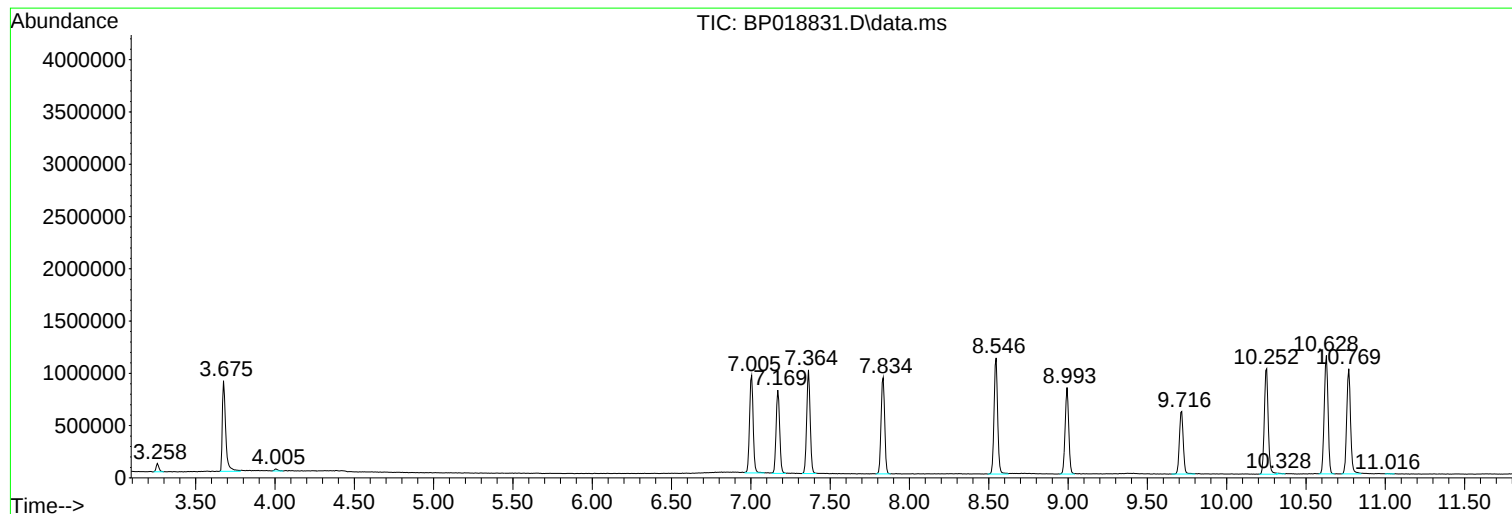

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018831.D
Acq On : 14 Dec 2023 06:31
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018831.D
Acq On : 14 Dec 2023 06:31
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc