

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018833.D
 Acq On : 14 Dec 2023 07:39
 Operator : MA/JU
 Sample : PB157726BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	38	rBV	75834	98885	1.53%	0.184%
2	3.675	96	100	117	rBV	865793	1270806	19.69%	2.359%
3	4.005	153	156	160	rVB2	13211	16707	0.26%	0.031%
4	7.005	659	666	676	rVB	905285	1419533	21.99%	2.635%
5	7.169	688	694	704	rVB	793661	1199457	18.58%	2.227%
6	7.363	719	727	739	rBV	954459	1474505	22.85%	2.737%
7	7.834	797	807	819	rBV	810666	1281467	19.85%	2.379%
8	8.546	918	928	942	rBV	1068661	1739696	26.95%	3.229%
9	8.993	997	1004	1012	rBV	815170	1293478	20.04%	2.401%
10	9.410	1074	1075	1086	rVB8	7522	13708	0.21%	0.025%
11	9.710	1118	1126	1136	rBV	580451	957759	14.84%	1.778%
12	10.246	1208	1217	1231	rBV	1009815	1701863	26.37%	3.159%
13	10.628	1273	1282	1291	rVB	994965	1637557	25.37%	3.040%
14	10.769	1298	1306	1321	rBV	976049	1691365	26.21%	3.140%
15	11.628	1443	1452	1457	rBV	3013	8300	0.13%	0.015%
16	12.216	1545	1552	1560	rBV2	18487	33695	0.52%	0.063%
17	12.834	1652	1657	1662	rBV7	5958	10544	0.16%	0.020%
18	13.369	1744	1748	1754	rVB4	17385	26361	0.41%	0.049%
19	13.881	1828	1835	1846	rBV	1704025	2337551	36.22%	4.339%
20	14.157	1874	1882	1898	rBV	1900644	2783835	43.13%	5.168%
21	14.463	1925	1934	1949	rBV	1367184	2042602	31.65%	3.792%
22	14.669	1962	1969	1988	rBV	627128	1101901	17.07%	2.045%
23	15.451	2095	2102	2112	rBV	2530748	3626296	56.18%	6.732%
24	15.575	2117	2123	2136	rVV	574276	816248	12.65%	1.515%
25	15.692	2140	2143	2146	rVB4	10492	14179	0.22%	0.026%
26	16.698	2310	2314	2316	rVB5	5841	8167	0.13%	0.015%
27	17.210	2395	2401	2411	rBV	1783273	2448558	37.94%	4.545%
28	17.310	2411	2418	2430	rBV	2944235	4199508	65.07%	7.796%
29	18.104	2548	2553	2560	rBV10	17363	33665	0.52%	0.062%
30	19.122	2723	2726	2731	rBV2	39402	47057	0.73%	0.087%
31	19.192	2734	2738	2744	rVV	36923	48276	0.75%	0.090%
32	19.545	2792	2798	2809	rBV	4214901	5388410	83.49%	10.003%
33	21.298	3091	3096	3103	rBV	2652233	3162229	48.99%	5.870%
34	23.504	3464	3471	3488	rVB2	3336769	6454285	100.00%	11.981%
35	23.657	3491	3497	3508	rVB	1769955	3481342	53.94%	6.463%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018833.D
Acq On : 14 Dec 2023 07:39
Operator : MA/JU
Sample : PB157726BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53869795

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018833.D
Acq On : 14 Dec 2023 07:39
Operator : MA/JU
Sample : PB157726BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

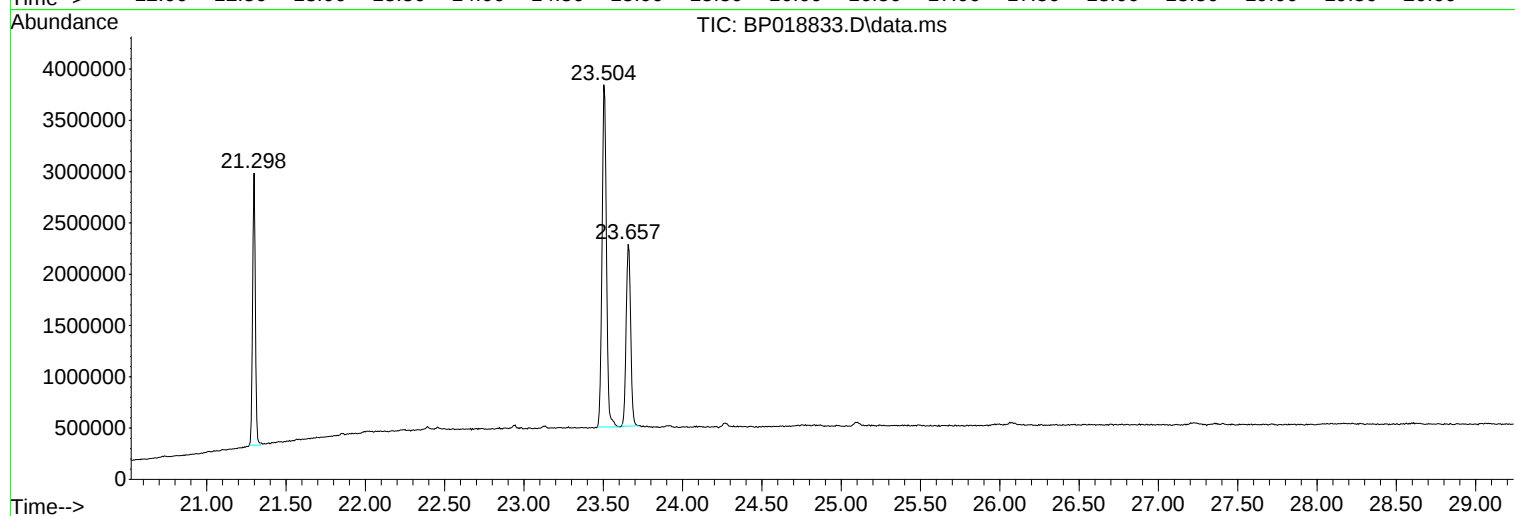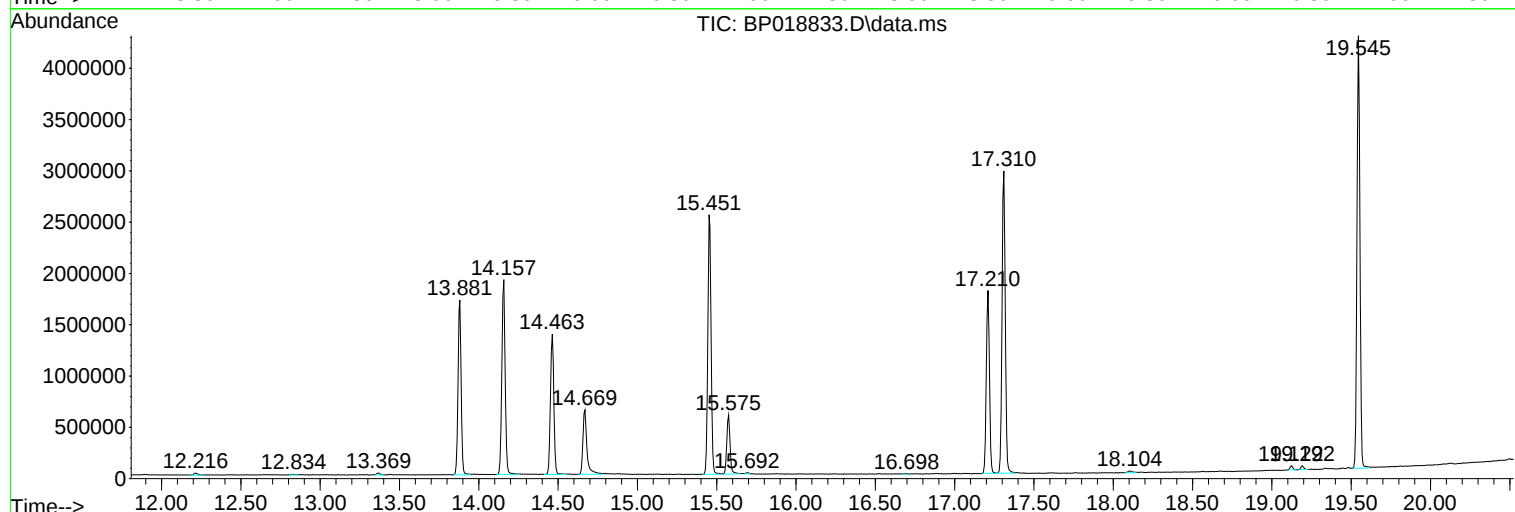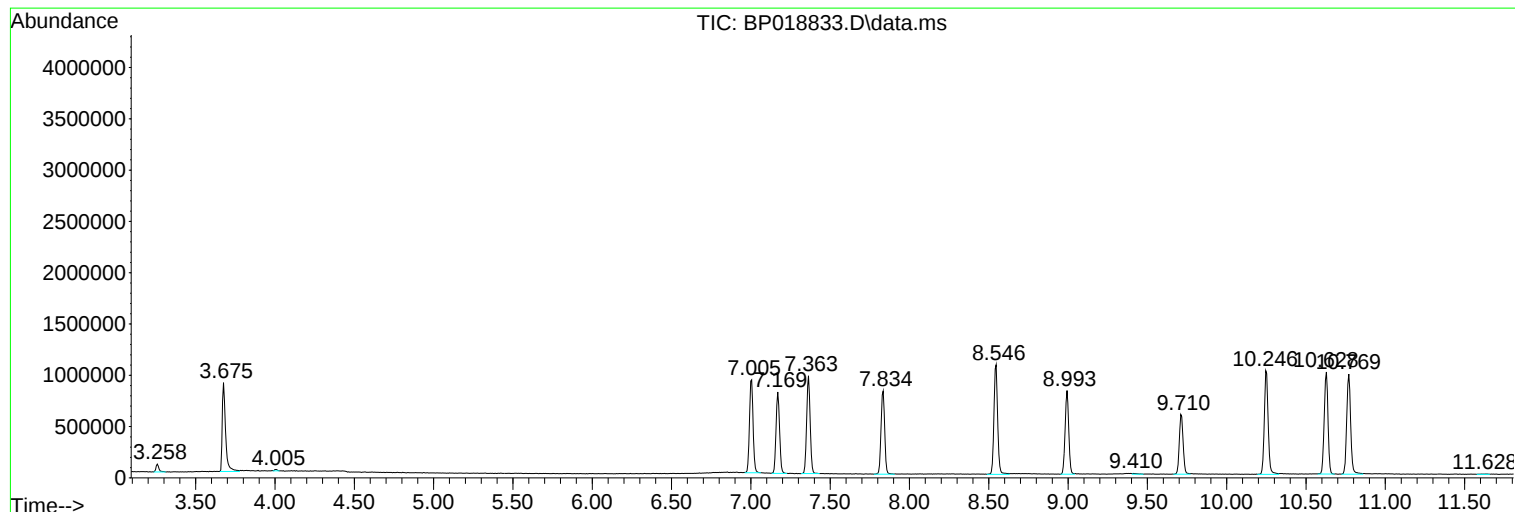

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018833.D
Acq On : 14 Dec 2023 07:39
Operator : MA/JU
Sample : PB157726BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018833.D
Acq On : 14 Dec 2023 07:39
Operator : MA/JU
Sample : PB157726BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc