

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018834.D
 Acq On : 14 Dec 2023 09:21
 Operator : MA/JU
 Sample : 05677-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	19	24	27	rBV	55055	79696	1.08%	0.137%
2	3.257	27	29	33	rVV	57120	71148	0.97%	0.123%
3	3.293	33	35	42	rVB	43034	51195	0.69%	0.088%
4	3.681	97	101	114	rBV	312940	479450	6.51%	0.826%
5	3.910	137	140	147	rVB2	20316	33401	0.45%	0.058%
6	4.010	154	157	162	rVB	18486	23697	0.32%	0.041%
7	4.540	241	247	256	rBV	351317	519562	7.05%	0.895%
8	5.534	412	416	421	rBV6	4820	8527	0.12%	0.015%
9	6.763	618	625	627	rBV7	5962	11800	0.16%	0.020%
10	7.004	660	666	675	rVB	205956	319271	4.33%	0.550%
11	7.169	686	694	703	rVB	874837	1349995	18.32%	2.326%
12	7.281	710	713	717	rVB4	5272	7400	0.10%	0.013%
13	7.363	720	727	738	rVB	844083	1293820	17.56%	2.230%
14	7.457	738	743	747	rBV8	6056	8839	0.12%	0.015%
15	7.834	799	807	817	rBV	973966	1515957	20.57%	2.612%
16	8.545	920	928	941	rBV	597548	958618	13.01%	1.652%
17	8.992	995	1004	1012	rBV	945377	1504873	20.42%	2.593%
18	9.104	1020	1023	1027	rBV6	4941	7491	0.10%	0.013%
19	9.404	1070	1074	1080	rVB9	5405	11509	0.16%	0.020%
20	9.716	1118	1127	1136	rBV	677691	1116041	15.14%	1.923%
21	10.251	1208	1218	1227	rBV	1057208	1785462	24.23%	3.077%
22	10.498	1253	1260	1263	rVB8	7326	16044	0.22%	0.028%
23	10.628	1275	1282	1290	rBV	1184550	1919799	26.05%	3.308%
24	10.769	1298	1306	1319	rBV	945500	1609935	21.85%	2.774%
25	11.016	1343	1348	1353	rVB9	5531	11371	0.15%	0.020%
26	12.051	1517	1524	1529	rVB10	4103	10442	0.14%	0.018%
27	12.216	1547	1552	1556	rBV2	19365	31933	0.43%	0.055%
28	12.410	1578	1585	1593	rVB2	5676	12329	0.17%	0.021%
29	12.833	1652	1657	1660	rBV6	7295	11991	0.16%	0.021%
30	13.069	1694	1697	1704	rVB8	6065	10950	0.15%	0.019%
31	13.257	1724	1729	1733	rBV8	6739	14134	0.19%	0.024%
32	13.363	1742	1747	1754	rVB6	16586	24939	0.34%	0.043%
33	13.880	1828	1835	1846	rBV	1813983	2576775	34.97%	4.441%
34	14.157	1874	1882	1895	rBV	2271852	3324954	45.12%	5.730%
35	14.463	1927	1934	1942	rBV	1668181	2417616	32.81%	4.166%
36	14.669	1963	1969	1983	rBV	86794	204865	2.78%	0.353%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018834.D
 Acq On : 14 Dec 2023 09:21
 Operator : MA/JU
 Sample : 05677-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.880	1999	2005	2011	rVB	7378	15263	0.21%	0.026%
38	15.451	2096	2102	2116	rBV	2776766	4212820	57.17%	7.260%
39	15.574	2116	2123	2134	rVV	594538	843809	11.45%	1.454%
40	15.698	2140	2144	2153	rVB3	17076	34703	0.47%	0.060%
41	16.233	2229	2235	2242	rVB3	7857	13645	0.19%	0.024%
42	16.398	2261	2263	2270	rVB8	5443	10420	0.14%	0.018%
43	16.692	2308	2313	2318	rBV9	5057	9699	0.13%	0.017%
44	16.886	2343	2346	2349	rBV5	5839	8564	0.12%	0.015%
45	17.210	2394	2401	2408	rBV	2067341	2878487	39.06%	4.961%
46	17.310	2411	2418	2429	rBV	3295709	4601124	62.44%	7.929%
47	18.098	2548	2552	2561	rBV3	68897	110060	1.49%	0.190%
48	19.121	2723	2726	2731	rVB	45533	57490	0.78%	0.099%
49	19.192	2734	2738	2742	rBV	48178	63768	0.87%	0.110%
50	19.333	2759	2762	2767	rBV4	42885	56151	0.76%	0.097%
51	19.545	2792	2798	2805	rBV	4633576	6084589	82.57%	10.486%
52	21.298	3091	3096	3103	rBV	3146098	3880670	52.66%	6.688%
53	23.503	3464	3471	3486	rVB2	3615646	7369225	100.00%	12.700%
54	23.656	3490	3497	3509	rVB	2245930	4420925	59.99%	7.619%




Sum of corrected areas: 58027241

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018834.D
Acq On : 14 Dec 2023 09:21
Operator : MA/JU
Sample : 05677-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

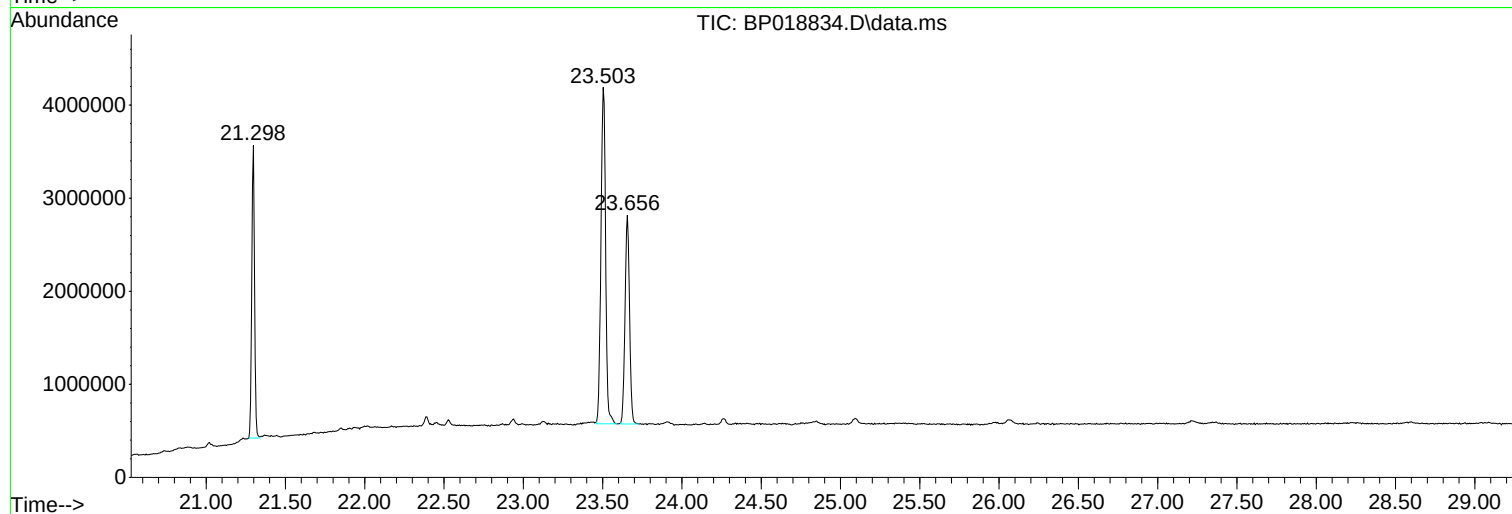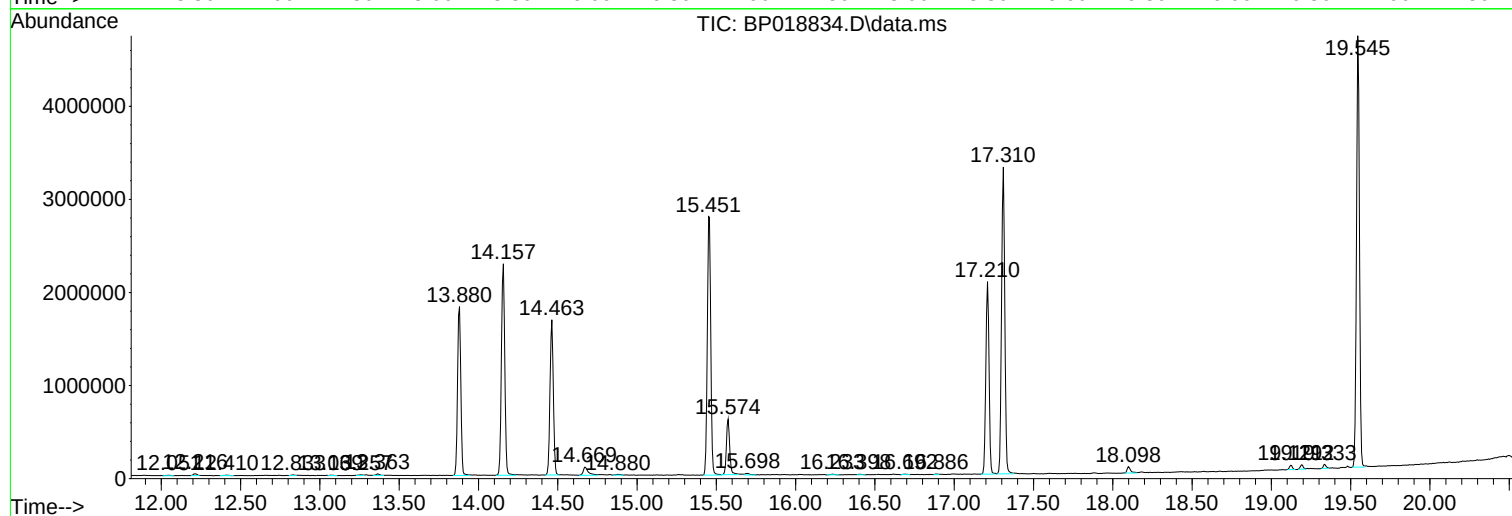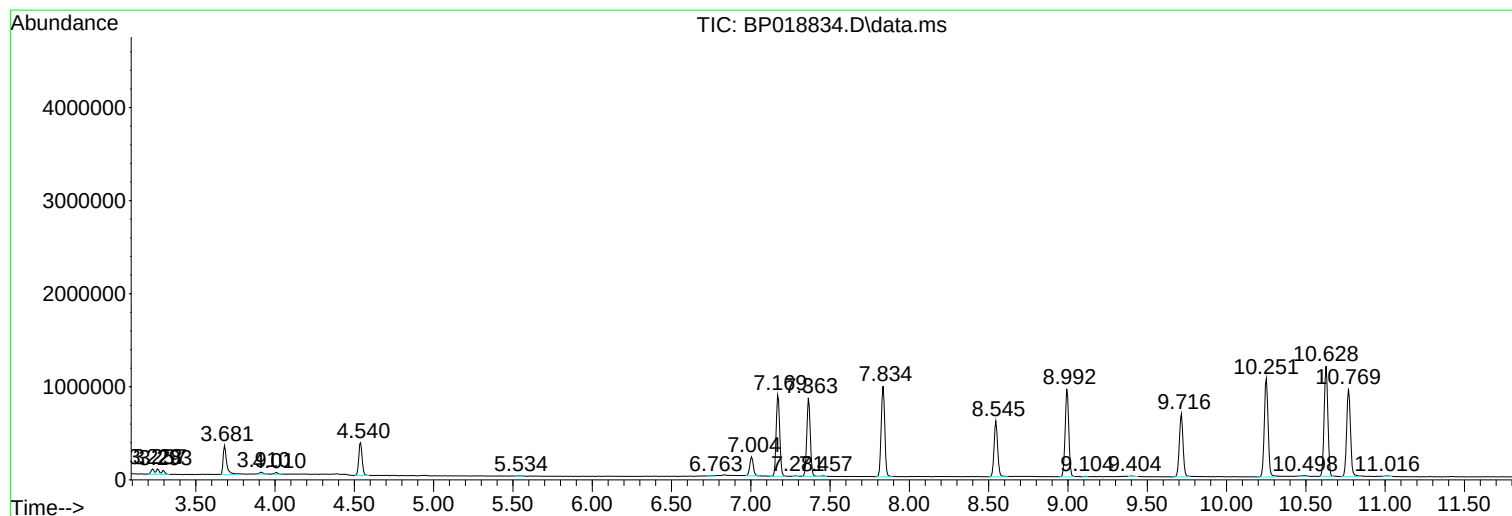

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018834.D
Acq On : 14 Dec 2023 09:21
Operator : MA/JU
Sample : 05677-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018834.D
Acq On : 14 Dec 2023 09:21
Operator : MA/JU
Sample : 05677-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc