

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018839.D
 Acq On : 14 Dec 2023 13:03
 Operator : MA/JU
 Sample : 05677-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	66436	81165	0.97%	0.148%
2	3.540	74	77	84	rBV	41050	62485	0.75%	0.114%
3	3.675	96	100	114	rBV	326121	518449	6.19%	0.948%
4	3.911	135	140	144	rVB2	22821	38449	0.46%	0.070%
5	4.005	153	156	159	rVB	13566	16689	0.20%	0.031%
6	4.534	241	246	251	rBV2	35228	53926	0.64%	0.099%
7	4.928	310	313	318	rVB6	7693	11624	0.14%	0.021%
8	5.111	342	344	352	rVB9	6402	10292	0.12%	0.019%
9	5.534	412	416	421	rBV6	5753	10458	0.12%	0.019%
10	6.999	658	665	680	rVB	196158	333586	3.99%	0.610%
11	7.169	687	694	704	rVB	729238	1126822	13.46%	2.061%
12	7.363	719	727	735	rBV	710399	1132826	13.53%	2.072%
13	7.452	735	742	747	rVB4	11107	21639	0.26%	0.040%
14	7.628	766	772	778	rVB4	6168	13157	0.16%	0.024%
15	7.828	799	806	814	rBV	736829	1174282	14.03%	2.148%
16	8.540	919	927	940	rBV	601819	984859	11.77%	1.802%
17	8.993	996	1004	1013	rBV	878028	1428074	17.06%	2.612%
18	9.410	1071	1075	1081	rVB7	9882	16359	0.20%	0.030%
19	9.569	1097	1102	1107	rVB7	8962	15553	0.19%	0.028%
20	9.710	1119	1126	1134	rBV	643240	1048654	12.53%	1.918%
21	10.246	1210	1217	1228	rBV	1050289	1709316	20.42%	3.127%
22	10.622	1273	1281	1289	rBV	864513	1462614	17.47%	2.676%
23	10.769	1296	1306	1316	rBV	831910	1443239	17.24%	2.640%
24	11.375	1404	1409	1416	rBV2	20020	39592	0.47%	0.072%
25	11.440	1416	1420	1428	rVB2	9412	20096	0.24%	0.037%
26	12.216	1546	1552	1557	rBV2	17590	29380	0.35%	0.054%
27	12.834	1651	1657	1659	rBV6	6168	12100	0.14%	0.022%
28	13.363	1742	1747	1754	rVV4	18904	33664	0.40%	0.062%
29	13.875	1828	1834	1846	rBV	1766110	2513967	30.03%	4.599%
30	14.151	1870	1881	1893	rBV	2054664	3035881	36.27%	5.554%
31	14.463	1926	1934	1943	rBV	1153785	1695676	20.26%	3.102%
32	14.669	1963	1969	1982	rVB	129559	242506	2.90%	0.444%
33	14.875	1999	2004	2011	rBV10	7674	20817	0.25%	0.038%
34	15.451	2096	2102	2109	rBV	2680258	3918782	46.81%	7.169%
35	15.575	2117	2123	2137	rBV	659765	963469	11.51%	1.763%
36	15.692	2137	2143	2150	rVB6	18375	41322	0.49%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018839.D
 Acq On : 14 Dec 2023 13:03
 Operator : MA/JU
 Sample : 05677-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.028	2194	2200	2203	rBV7	7570	13554	0.16%	0.025%
38	16.151	2217	2221	2222	rBV3	8991	10462	0.12%	0.019%
39	16.616	2298	2300	2306	rVB7	7465	9134	0.11%	0.017%
40	16.716	2314	2317	2322	rVB2	19703	28058	0.34%	0.051%
41	16.880	2342	2345	2349	rVB6	10069	13711	0.16%	0.025%
42	17.210	2394	2401	2411	rBV	1553777	2214600	26.46%	4.051%
43	17.310	2411	2418	2431	rVV	3479091	4928192	58.87%	9.015%
44	17.598	2463	2467	2474	rBV9	21750	48393	0.58%	0.089%
45	18.098	2548	2552	2560	rBV	124619	181137	2.16%	0.331%
46	18.175	2562	2565	2572	rVB2	31062	46850	0.56%	0.086%
47	19.122	2723	2726	2731	rVB	50384	62590	0.75%	0.114%
48	19.192	2734	2738	2742	rBV	59350	80212	0.96%	0.147%
49	19.333	2759	2762	2766	rBV2	69790	85591	1.02%	0.157%
50	19.545	2792	2798	2805	rBV	5096084	6851603	81.85%	12.534%
51	21.298	3091	3096	3102	rBV	2543375	3088009	36.89%	5.649%
52	23.510	3464	3472	3489	rVB2	4191559	8371037	100.00%	15.314%
53	23.657	3491	3497	3507	rVB	1644519	3348989	40.01%	6.127%




Sum of corrected areas: 54663891

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018839.D
Acq On : 14 Dec 2023 13:03
Operator : MA/JU
Sample : 05677-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

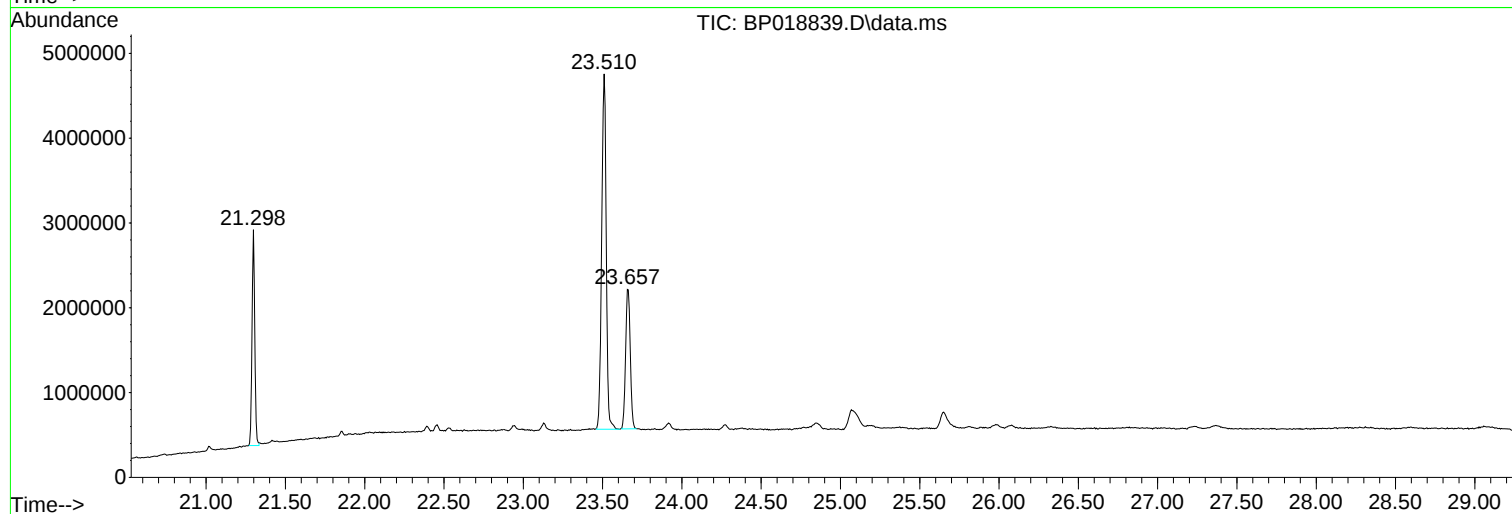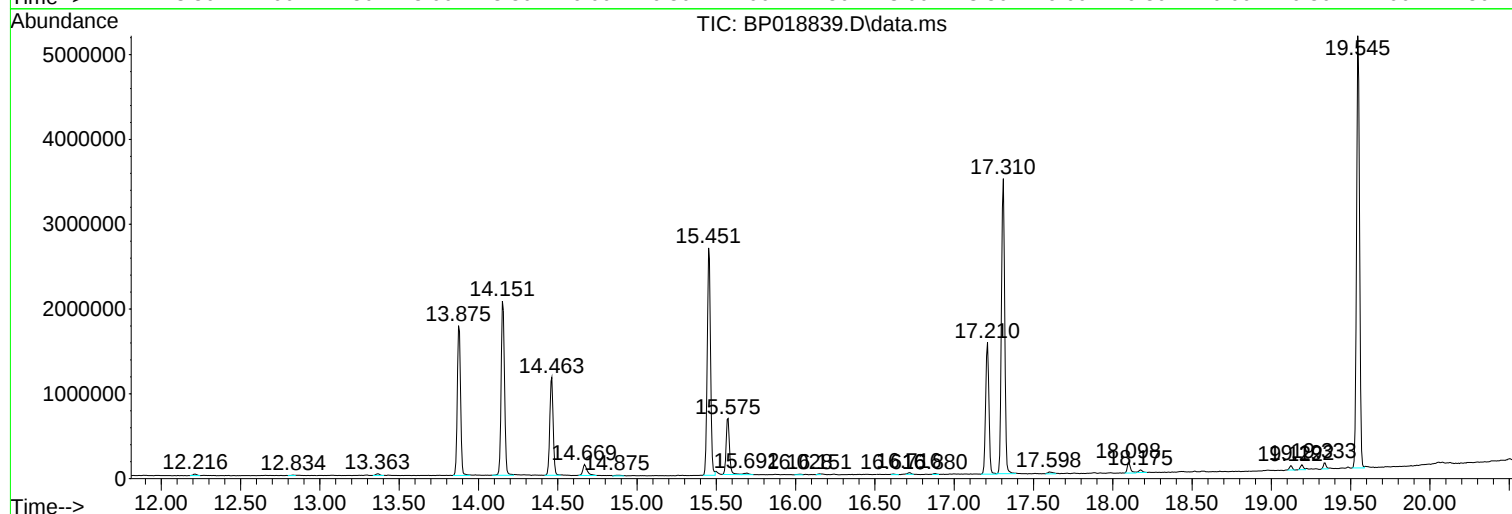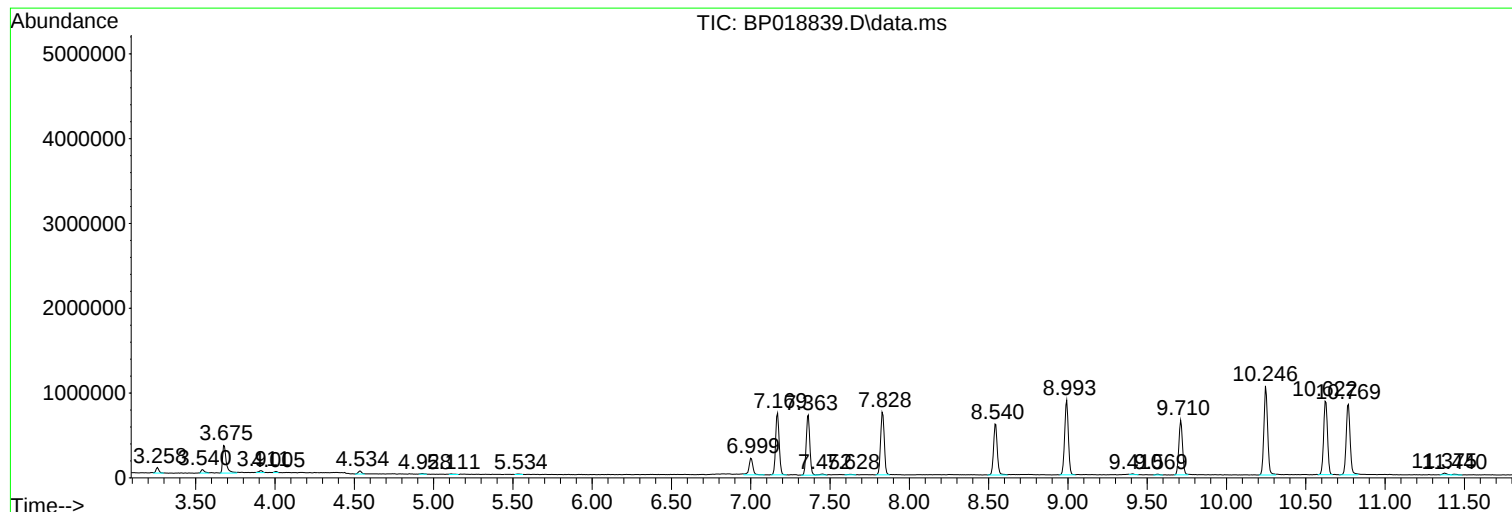

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018839.D
Acq On : 14 Dec 2023 13:03
Operator : MA/JU
Sample : 05677-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018839.D
Acq On : 14 Dec 2023 13:03
Operator : MA/JU
Sample : 05677-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc