

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018841.D
 Acq On : 14 Dec 2023 14:11
 Operator : MA/JU
 Sample : 05677-08
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.229	19	24	27	rBV	109569	163863	2.15%	0.279%
2	3.258	27	29	38	rVB	76869	96826	1.27%	0.165%
3	3.552	77	79	86	rVB3	6503	8508	0.11%	0.014%
4	3.681	97	101	111	rBV	363650	555848	7.30%	0.946%
5	3.911	136	140	146	rVB	27526	42317	0.56%	0.072%
6	4.005	153	156	161	rVB2	16384	21674	0.28%	0.037%
7	4.534	241	246	254	rBV	225936	319733	4.20%	0.544%
8	4.928	310	313	320	rVB3	9362	13838	0.18%	0.024%
9	7.005	660	666	677	rVB	310356	494087	6.49%	0.841%
10	7.169	687	694	707	rVB	979264	1512558	19.87%	2.573%
11	7.364	719	727	738	rBV	998160	1554817	20.43%	2.645%
12	7.458	738	743	746	rVV6	5797	9334	0.12%	0.016%
13	7.834	798	807	815	rBV	888897	1422759	18.69%	2.420%
14	8.540	921	927	938	rBV	753738	1227726	16.13%	2.089%
15	8.993	997	1004	1020	rBV	1021894	1632084	21.44%	2.777%
16	9.116	1020	1025	1035	rVV	43112	70142	0.92%	0.119%
17	9.393	1070	1072	1079	rVB6	4991	10154	0.13%	0.017%
18	9.569	1097	1102	1103	rBV5	7792	10175	0.13%	0.017%
19	9.711	1118	1126	1140	rVB	695280	1149113	15.10%	1.955%
20	10.246	1210	1217	1228	rBV	1151202	1954913	25.68%	3.326%
21	10.628	1274	1282	1295	rVB	1060212	1783733	23.43%	3.035%
22	10.769	1298	1306	1321	rBV	907130	1538071	20.21%	2.617%
23	11.375	1404	1409	1415	rBV7	11013	24011	0.32%	0.041%
24	11.963	1503	1509	1518	rBV2	35387	64443	0.85%	0.110%
25	12.216	1545	1552	1556	rBV	22265	39566	0.52%	0.067%
26	12.369	1572	1578	1580	rBV7	5428	10381	0.14%	0.018%
27	13.363	1742	1747	1755	rBV4	20620	33807	0.44%	0.058%
28	13.875	1826	1834	1848	rBV	1882503	2697656	35.44%	4.589%
29	14.157	1874	1882	1895	rBV	2254241	3394916	44.60%	5.776%
30	14.463	1927	1934	1942	rBV	1473583	2137069	28.08%	3.636%
31	14.675	1963	1970	1990	rBV3	187650	541251	7.11%	0.921%
32	14.928	2008	2013	2026	rVB	126623	198537	2.61%	0.338%
33	15.451	2096	2102	2109	rBV	2974169	4292468	56.39%	7.303%
34	15.575	2117	2123	2138	rVV	682895	953088	12.52%	1.621%
35	15.693	2140	2143	2152	rVB5	18472	29037	0.38%	0.049%
36	16.240	2232	2236	2239	rBV6	5673	7816	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018841.D
 Acq On : 14 Dec 2023 14:11
 Operator : MA/JU
 Sample : 05677-08
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.445	2266	2271	2282	rBV3	54161	91971	1.21%	0.156%
38	16.622	2296	2301	2307	rBV9	16703	28981	0.38%	0.049%
39	17.210	2394	2401	2407	rBV	1814095	2523818	33.16%	4.294%
40	17.310	2411	2418	2429	rVV	3206357	4688397	61.59%	7.976%
41	18.098	2548	2552	2559	rBV3	71555	100691	1.32%	0.171%
42	18.181	2561	2566	2575	rVV2	75962	119449	1.57%	0.203%
43	19.034	2708	2711	2715	rBV3	19924	27292	0.36%	0.046%
44	19.122	2722	2726	2730	rVB2	48165	62037	0.82%	0.106%
45	19.192	2734	2738	2742	rBV	50187	74959	0.98%	0.128%
46	19.334	2759	2762	2769	rBV5	52646	66268	0.87%	0.113%
47	19.545	2792	2798	2806	rBV	4590076	6153145	80.84%	10.468%
48	21.298	3091	3096	3101	rBV	2678647	3356591	44.10%	5.710%
49	23.504	3464	3471	3488	rVB2	3842546	7611762	100.00%	12.949%
50	23.657	3490	3497	3506	rVB	1955611	3859101	50.70%	6.565%




Sum of corrected areas: 58780781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018841.D
Acq On : 14 Dec 2023 14:11
Operator : MA/JU
Sample : 05677-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

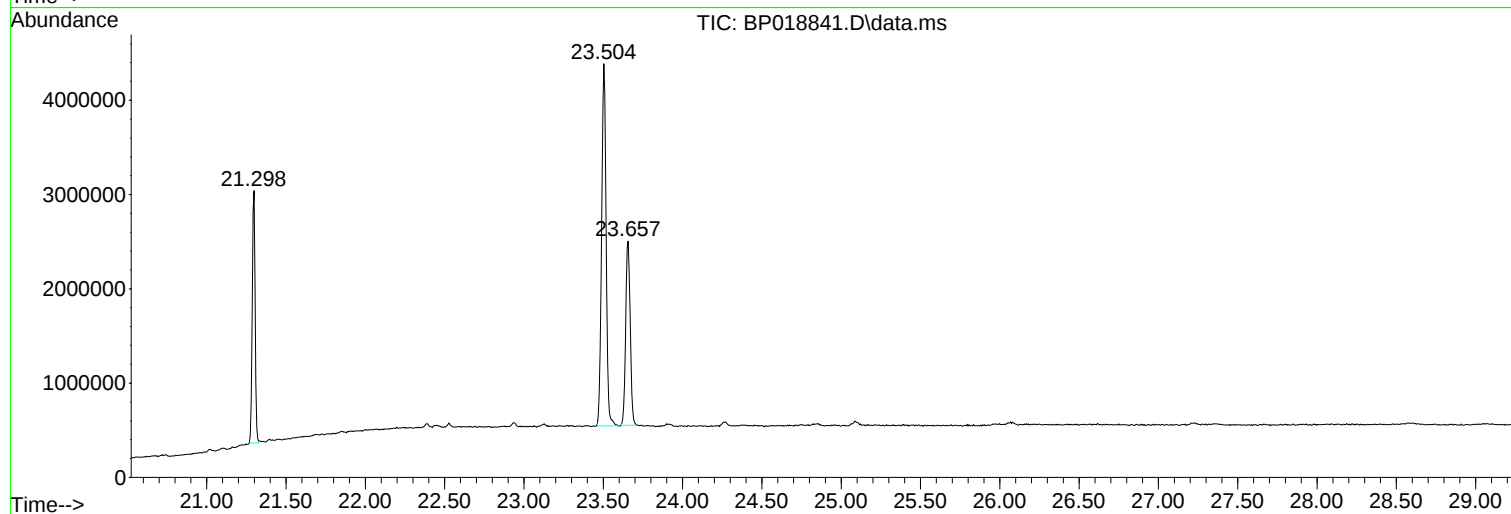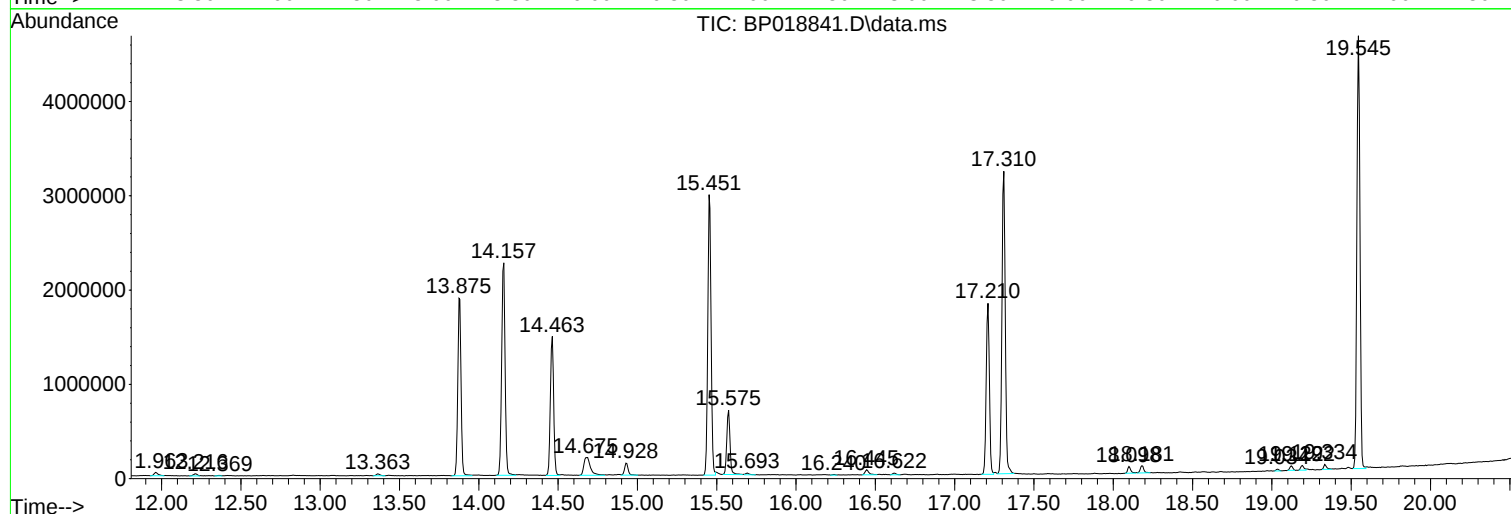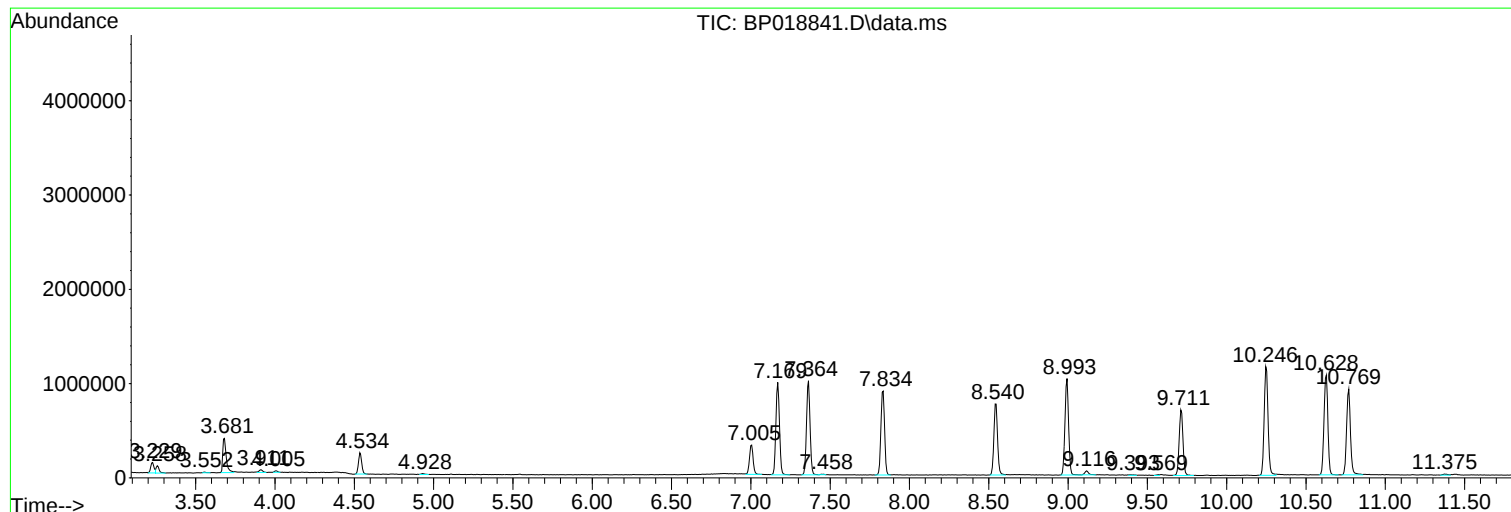

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018841.D
Acq On : 14 Dec 2023 14:11
Operator : MA/JU
Sample : 05677-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018841.D
Acq On : 14 Dec 2023 14:11
Operator : MA/JU
Sample : 05677-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc