

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018845.D
 Acq On : 14 Dec 2023 16:26
 Operator : MA/JU
 Sample : PB157639BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	35	rVB	66373	81203	1.51%	0.183%
2	3.675	96	100	115	rBV	758468	1102631	20.55%	2.489%
3	4.005	153	156	161	rVB3	12357	17006	0.32%	0.038%
4	7.005	659	666	676	rVB	723199	1126407	21.00%	2.542%
5	7.169	688	694	705	rVB	593157	912539	17.01%	2.060%
6	7.363	720	727	736	rBV	660638	1041228	19.41%	2.350%
7	7.834	799	807	817	rBV	704853	1126374	20.99%	2.542%
8	8.546	919	928	939	rBV	892627	1452270	27.07%	3.278%
9	8.993	996	1004	1012	rBV	668173	1066900	19.89%	2.408%
10	9.710	1118	1126	1137	rBV	500803	808708	15.07%	1.825%
11	10.246	1210	1217	1237	rBV	813679	1426874	26.60%	3.220%
12	10.481	1253	1257	1263	rVB8	6134	12128	0.23%	0.027%
13	10.628	1275	1282	1292	rVB	844063	1405620	26.20%	3.172%
14	10.769	1297	1306	1324	rBV	832032	1457653	27.17%	3.290%
15	11.887	1492	1496	1498	rBV5	4862	6649	0.12%	0.015%
16	12.216	1545	1552	1558	rVB4	15595	26832	0.50%	0.061%
17	12.828	1649	1656	1659	rBV8	3165	6096	0.11%	0.014%
18	13.369	1741	1748	1753	rBV8	7780	13314	0.25%	0.030%
19	13.434	1755	1759	1764	rVV8	4300	7311	0.14%	0.017%
20	13.510	1767	1772	1775	rBV6	3018	5591	0.10%	0.013%
21	13.651	1791	1796	1800	rVB3	6575	12306	0.23%	0.028%
22	13.875	1828	1834	1847	rBV	1080371	1531143	28.54%	3.456%
23	14.151	1873	1881	1890	rBV	1391077	2045049	38.12%	4.616%
24	14.463	1927	1934	1941	rBV	1132275	1686434	31.43%	3.806%
25	14.669	1962	1969	1989	rBV	459676	851077	15.86%	1.921%
26	15.240	2063	2066	2069	rBV5	3480	6335	0.12%	0.014%
27	15.451	2096	2102	2113	rBV	2068404	2947242	54.93%	6.652%
28	15.575	2117	2123	2136	rVV	427376	625961	11.67%	1.413%
29	15.698	2140	2144	2148	rVB6	10813	16825	0.31%	0.038%
30	16.786	2324	2329	2330	rBV5	3485	6009	0.11%	0.014%
31	16.992	2360	2364	2366	rBV5	5170	7504	0.14%	0.017%
32	17.210	2394	2401	2411	rBV	1492064	2088910	38.94%	4.715%
33	17.310	2411	2418	2429	rBV	2314185	3370251	62.82%	7.607%
34	18.098	2548	2552	2556	rBV6	20915	33076	0.62%	0.075%
35	19.122	2723	2726	2733	rVB2	34108	41558	0.77%	0.094%
36	19.192	2734	2738	2743	rBV	33551	47915	0.89%	0.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018845.D
Acq On : 14 Dec 2023 16:26
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK639

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.545	2792	2798	2805	rBV	3510676	4514902	84.16%	10.190%
38	21.298	3091	3096	3105	rBV	2293003	2858102	53.27%	6.451%
39	23.504	3464	3471	3486	rVB2	2720603	5364970	100.00%	12.109%
40	23.657	3491	3497	3508	rVB	1622643	3147830	58.67%	7.105%




Sum of corrected areas: 44306733

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018845.D
Acq On : 14 Dec 2023 16:26
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

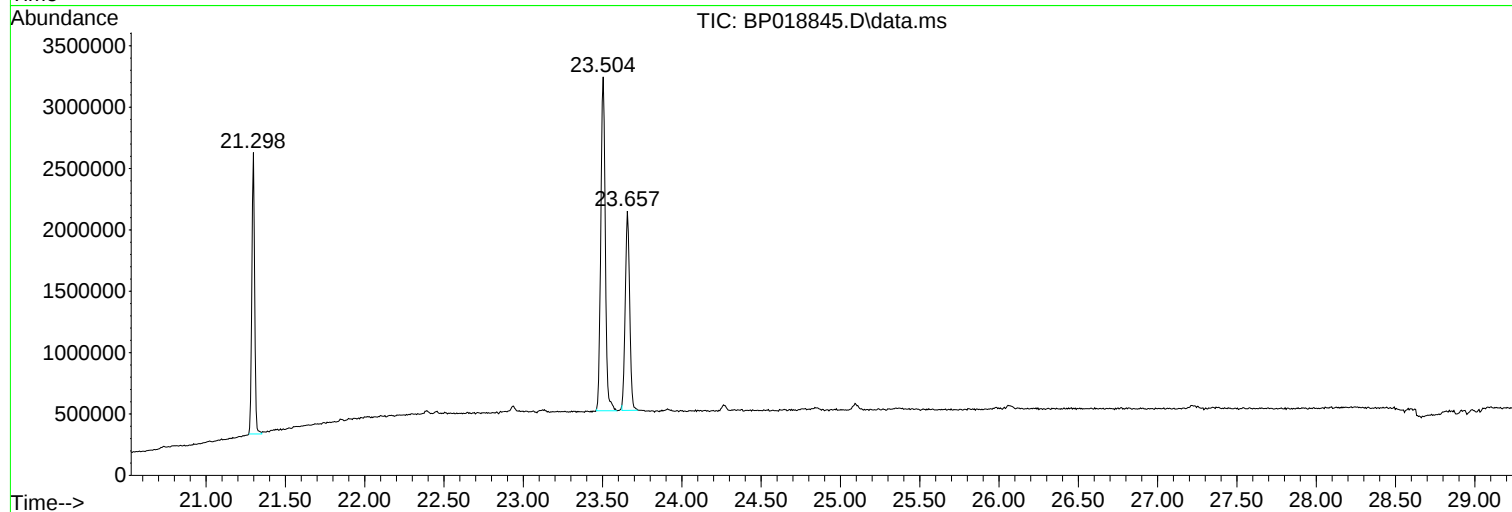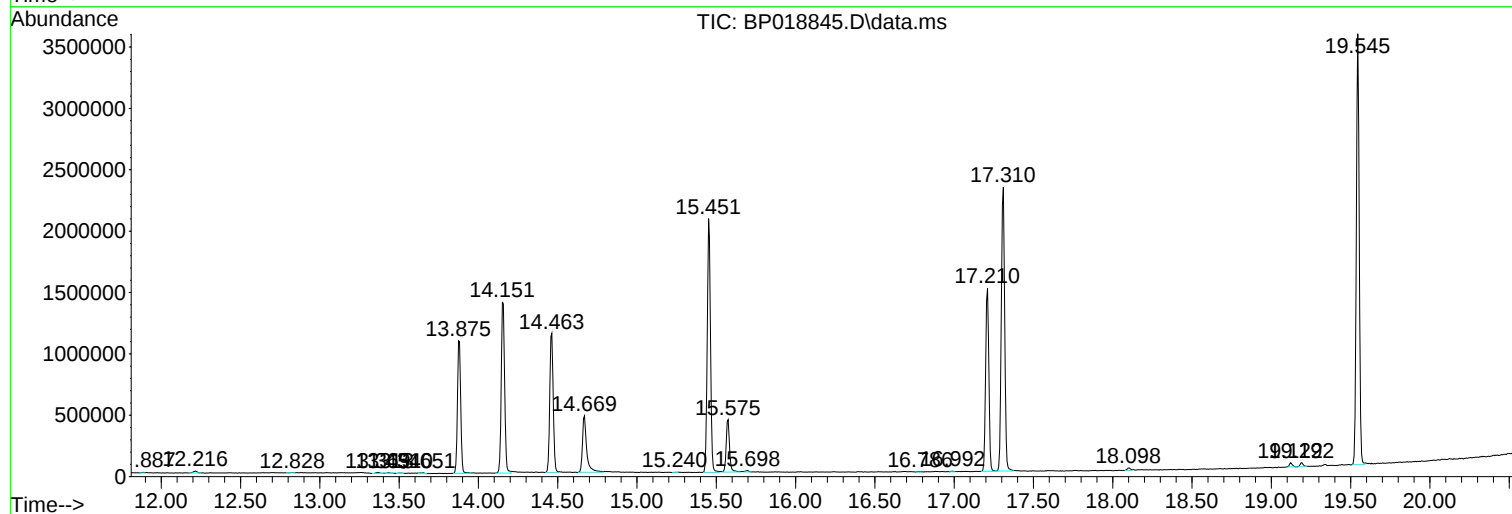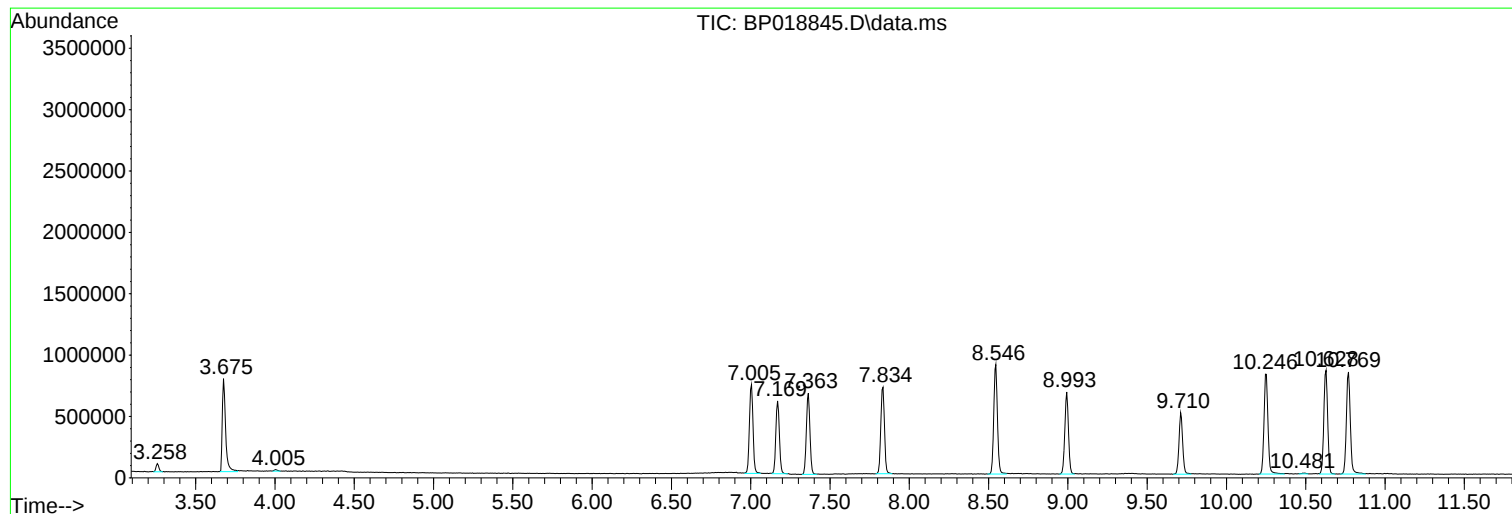

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018845.D
Acq On : 14 Dec 2023 16:26
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018845.D
Acq On : 14 Dec 2023 16:26
Operator : MA/JU
Sample : PB157639BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc