

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018846.D
 Acq On : 14 Dec 2023 17:01
 Operator : MA/JU
 Sample : PB157722BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK722

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	34	rVB	73664	88925	1.48%	0.178%
2	3.675	96	100	118	rBV	795360	1163945	19.43%	2.336%
3	4.005	153	156	164	rVB	17300	24311	0.41%	0.049%
4	7.005	659	666	677	rVB	858585	1325659	22.13%	2.661%
5	7.169	688	694	703	rVB	742169	1099268	18.35%	2.206%
6	7.363	720	727	737	rBV	896039	1386932	23.15%	2.784%
7	7.834	800	807	816	rVB	840696	1331106	22.22%	2.672%
8	8.546	921	928	938	rBV	851503	1353324	22.59%	2.716%
9	8.993	996	1004	1014	rBV	561510	900477	15.03%	1.807%
10	9.710	1117	1126	1136	rBV	451353	745367	12.44%	1.496%
11	10.251	1210	1218	1235	rBV	891708	1552614	25.92%	3.116%
12	10.628	1274	1282	1291	rVB	1005400	1665863	27.81%	3.344%
13	10.769	1296	1306	1325	rBV	862638	1510010	25.21%	3.031%
14	11.898	1494	1498	1502	rVB7	3789	6885	0.11%	0.014%
15	12.210	1547	1551	1559	rVB2	16758	27837	0.46%	0.056%
16	13.251	1726	1728	1733	rBV6	3673	6827	0.11%	0.014%
17	13.369	1743	1748	1753	rBV5	14531	24589	0.41%	0.049%
18	13.881	1828	1835	1845	rBV	1495502	2032072	33.92%	4.079%
19	14.157	1874	1882	1891	rBV	1640355	2442196	40.77%	4.902%
20	14.463	1927	1934	1942	rBV	1378787	2004671	33.46%	4.024%
21	14.669	1962	1969	1988	rBV	556263	979660	16.35%	1.966%
22	15.451	2096	2102	2112	rBV	2165087	3166636	52.86%	6.356%
23	15.575	2117	2123	2132	rVV	513426	711854	11.88%	1.429%
24	15.692	2140	2143	2151	rVB5	12137	19413	0.32%	0.039%
25	16.686	2308	2312	2317	rBV7	7115	13294	0.22%	0.027%
26	17.210	2394	2401	2408	rBV	1778697	2448577	40.88%	4.915%
27	17.310	2411	2418	2431	rVV	2610891	3710423	61.94%	7.447%
28	17.622	2468	2471	2474	rBV4	4898	6047	0.10%	0.012%
29	18.104	2548	2553	2557	rBV6	17890	27804	0.46%	0.056%
30	19.122	2723	2726	2731	rVB2	36199	49901	0.83%	0.100%
31	19.192	2734	2738	2744	rBV	36474	49892	0.83%	0.100%
32	19.333	2760	2762	2767	rVB6	12615	15970	0.27%	0.032%
33	19.545	2792	2798	2805	rBV	3859427	4997160	83.42%	10.030%
34	21.298	3091	3096	3104	rBV	2658763	3301062	55.11%	6.626%
35	23.504	3464	3471	3479	rBV2	3051278	5990373	100.00%	12.023%
36	23.662	3491	3498	3508	rVB	1795238	3642176	60.80%	7.310%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018846.D
Acq On : 14 Dec 2023 17:01
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 49823120

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018846.D
Acq On : 14 Dec 2023 17:01
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

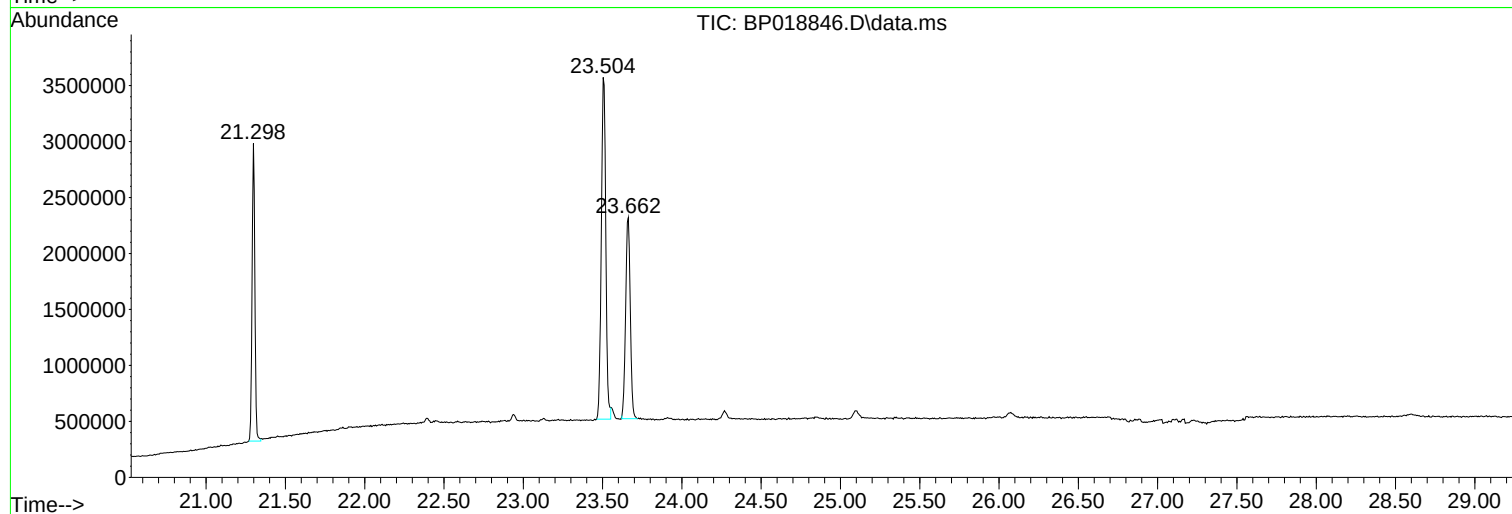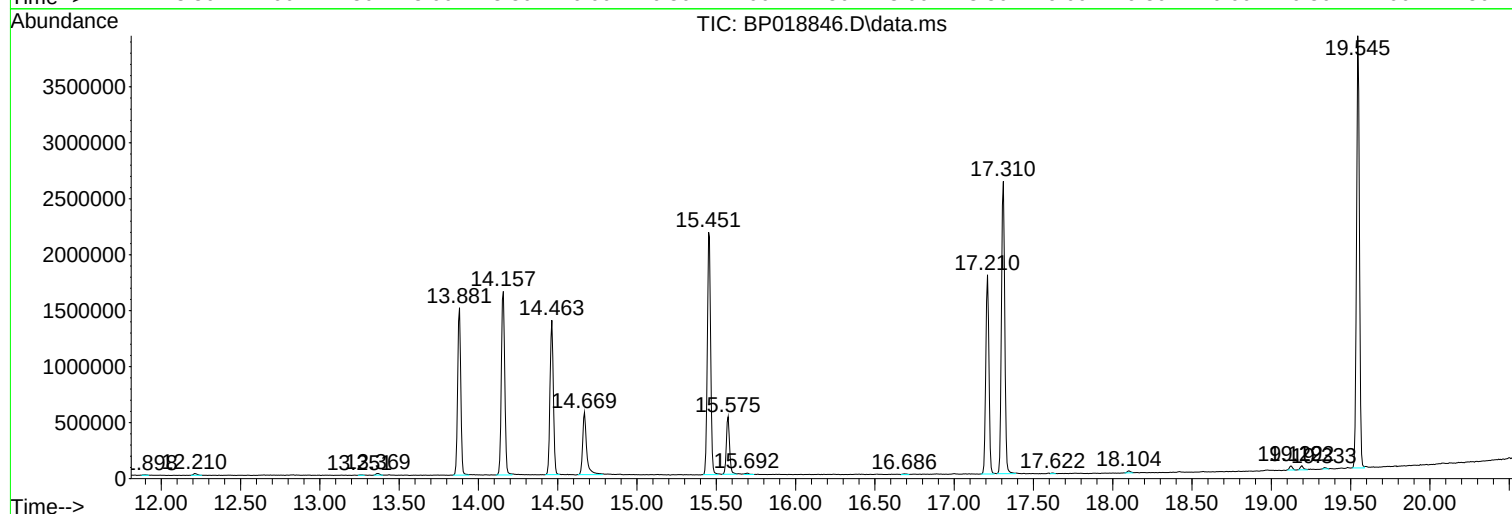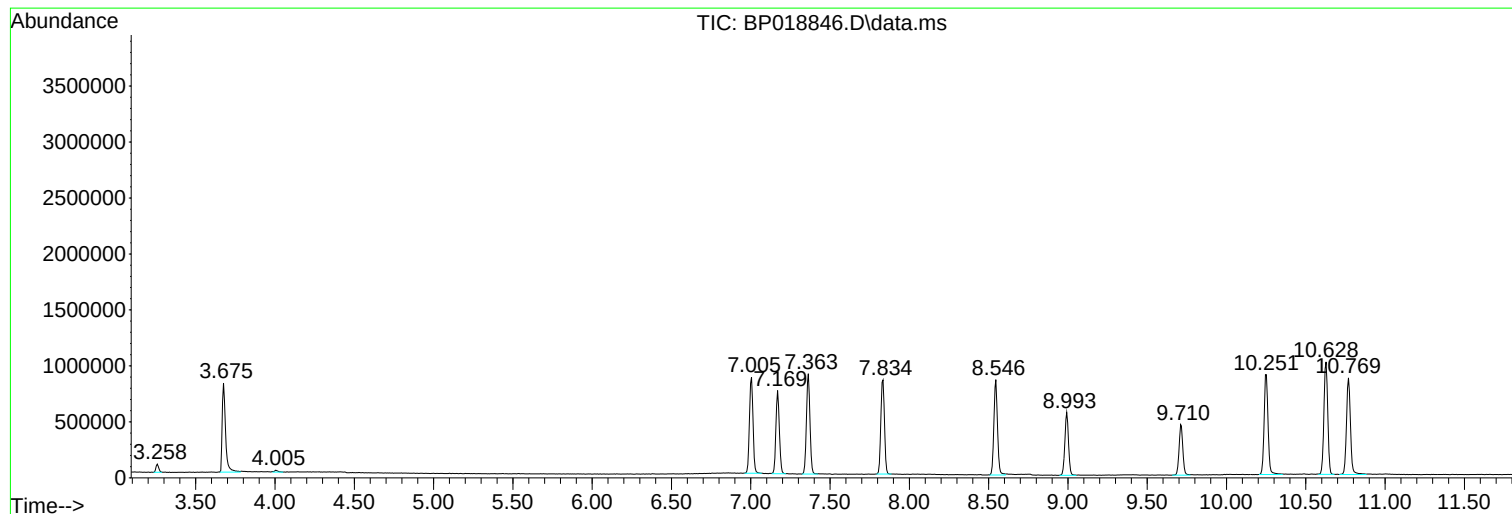

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018846.D
Acq On : 14 Dec 2023 17:01
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018846.D
Acq On : 14 Dec 2023 17:01
Operator : MA/JU
Sample : PB157722BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK722

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc