

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018847.D
 Acq On : 14 Dec 2023 17:35
 Operator : MA/JU
 Sample : 05677-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	18	23	27	rBV	308866	438699	8.14%	1.016%
2	3.681	97	101	111	rBV	238326	374277	6.95%	0.867%
3	4.005	154	156	161	rVB2	13995	16744	0.31%	0.039%
4	4.534	240	246	254	rBV	1363578	1942257	36.05%	4.498%
5	4.928	311	313	319	rVB4	7099	9415	0.17%	0.022%
6	5.111	340	344	349	rVB5	5987	7920	0.15%	0.018%
7	5.722	444	448	452	rVB	8976	11838	0.22%	0.027%
8	7.005	660	666	673	rVB	171169	267405	4.96%	0.619%
9	7.169	688	694	708	rVB	716312	1092478	20.28%	2.530%
10	7.275	708	712	716	rVV4	7444	11863	0.22%	0.027%
11	7.364	720	727	735	rVV	674261	1045379	19.40%	2.421%
12	7.458	739	743	749	rVB7	5067	9135	0.17%	0.021%
13	7.834	798	807	816	rBV	603284	966480	17.94%	2.238%
14	8.546	921	928	937	rBV	471764	759996	14.11%	1.760%
15	8.987	997	1003	1013	rVB	623023	1025065	19.03%	2.374%
16	9.116	1020	1025	1029	rBV8	3209	6351	0.12%	0.015%
17	9.293	1049	1055	1058	rBV8	2494	6108	0.11%	0.014%
18	9.334	1058	1062	1063	rVV4	5146	6529	0.12%	0.015%
19	9.375	1067	1069	1072	rVV4	7495	11135	0.21%	0.026%
20	9.405	1072	1074	1080	rVB6	7363	11584	0.22%	0.027%
21	9.710	1119	1126	1134	rBV	401281	652951	12.12%	1.512%
22	10.246	1209	1217	1229	rBV	622815	1062675	19.72%	2.461%
23	10.628	1275	1282	1290	rVB	523078	895040	16.61%	2.073%
24	10.769	1298	1306	1324	rBV	513185	892306	16.56%	2.067%
25	11.440	1415	1420	1427	rVB	4231	10577	0.20%	0.024%
26	11.899	1492	1498	1502	rVB4	8725	15255	0.28%	0.035%
27	12.210	1547	1551	1557	rVB2	12457	19427	0.36%	0.045%
28	12.422	1583	1587	1592	rBV6	3309	6721	0.12%	0.016%
29	13.369	1741	1748	1753	rBV4	14852	31514	0.58%	0.073%
30	13.881	1828	1835	1849	rBV	1463272	2055075	38.14%	4.759%
31	14.157	1875	1882	1895	rBV	1699987	2520469	46.78%	5.837%
32	14.463	1927	1934	1942	rBV	992022	1491341	27.68%	3.454%
33	14.522	1942	1944	1947	rVB4	4991	6008	0.11%	0.014%
34	14.675	1964	1970	1981	rBV2	74493	170414	3.16%	0.395%
35	14.863	1998	2002	2010	rVV5	8091	20402	0.38%	0.047%
36	14.934	2011	2014	2017	rVB5	6641	8212	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018847.D
 Acq On : 14 Dec 2023 17:35
 Operator : MA/JU
 Sample : 05677-09
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.245	2063	2067	2069	rBV5	3689	6061	0.11%	0.014%
38	15.451	2096	2102	2108	rVV	2251355	3263660	60.58%	7.558%
39	15.504	2108	2111	2116	rVV2	39214	70790	1.31%	0.164%
40	15.575	2117	2123	2138	rVV	512901	731289	13.57%	1.694%
41	15.692	2140	2143	2151	rVB4	13177	21806	0.40%	0.051%
42	16.616	2297	2300	2306	rVB7	10535	16036	0.30%	0.037%
43	17.028	2368	2370	2374	rVB5	6194	6318	0.12%	0.015%
44	17.210	2394	2401	2406	rBV	1277066	1832850	34.02%	4.245%
45	17.251	2406	2408	2412	rVV	64704	73541	1.37%	0.170%
46	17.310	2412	2418	2430	rVV	2560449	3660641	67.95%	8.478%
47	18.098	2548	2552	2557	rBV	122575	164295	3.05%	0.380%
48	18.157	2558	2562	2564	rBV	81242	102356	1.90%	0.237%
49	19.122	2722	2726	2732	rBV3	38655	53995	1.00%	0.125%
50	19.192	2734	2738	2740	rBV2	40501	51839	0.96%	0.120%
51	19.333	2759	2762	2768	rBV4	53120	68224	1.27%	0.158%
52	19.545	2792	2798	2805	rBV	3878035	4884155	90.66%	11.311%
53	21.298	3091	3096	3101	rBV	1864585	2352804	43.67%	5.449%
54	23.504	3464	3471	3484	rVB2	2718797	5387614	100.00%	12.477%
55	23.657	3491	3497	3507	rVB	1268734	2552155	47.37%	5.911%




Sum of corrected areas: 43179474

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018847.D
Acq On : 14 Dec 2023 17:35
Operator : MA/JU
Sample : 05677-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

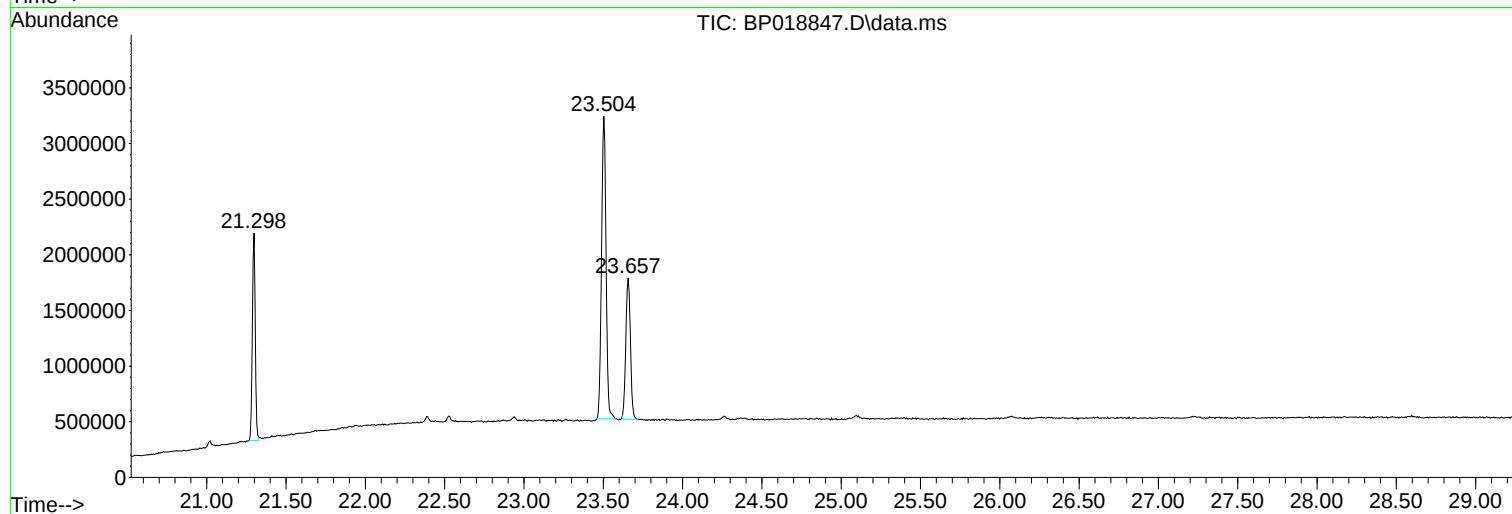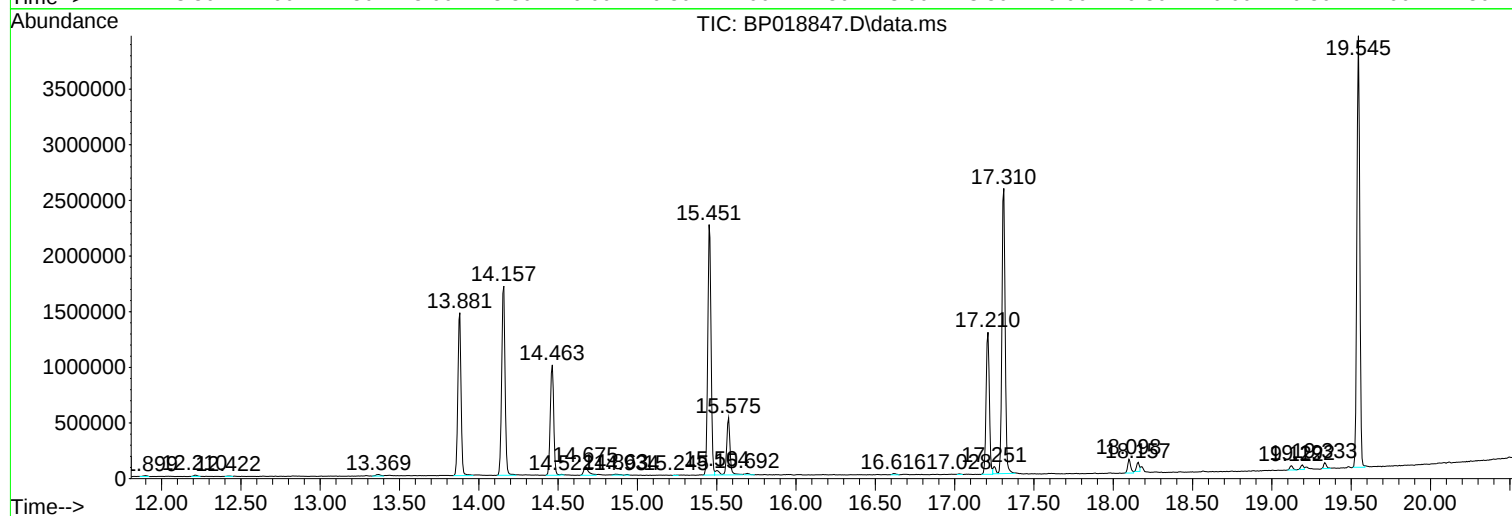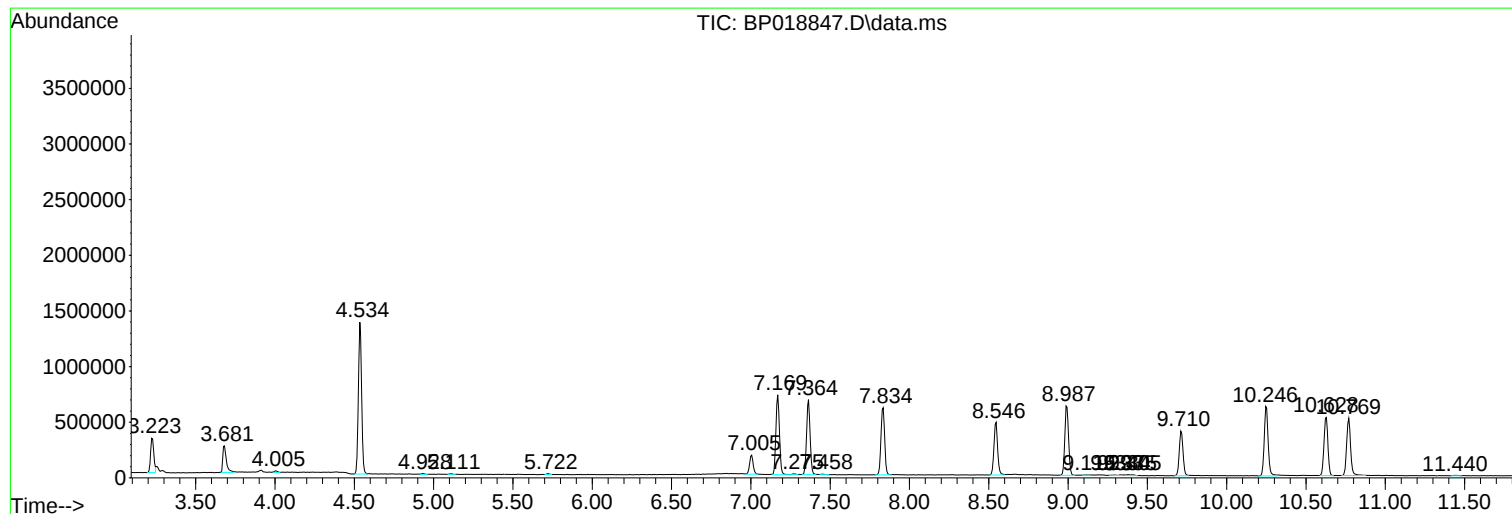

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018847.D
Acq On : 14 Dec 2023 17:35
Operator : MA/JU
Sample : 05677-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018847.D
Acq On : 14 Dec 2023 17:35
Operator : MA/JU
Sample : 05677-09
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc