

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018850.D
 Acq On : 14 Dec 2023 19:16
 Operator : MA/JU
 Sample : 05627-19DL 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	99	102	112	rBV	40451	74143	1.46%	0.276%
2	4.005	154	156	162	rVB2	15510	19347	0.38%	0.072%
3	7.005	662	666	672	rVB2	17405	28452	0.56%	0.106%
4	7.169	688	694	706	rVB	111090	180780	3.56%	0.673%
5	7.363	721	727	736	rVB	57606	101167	1.99%	0.376%
6	7.463	742	744	749	rVB5	6042	8400	0.17%	0.031%
7	7.834	799	807	816	rVB	768554	1287026	25.31%	4.788%
8	7.910	816	820	826	rBV8	6950	12292	0.24%	0.046%
9	8.063	840	846	848	rBV7	4061	7101	0.14%	0.026%
10	8.546	922	928	935	rBV	50396	85510	1.68%	0.318%
11	8.993	998	1004	1012	rVB	105209	169779	3.34%	0.632%
12	9.710	1120	1126	1132	rBV2	41024	72182	1.42%	0.269%
13	10.252	1211	1218	1226	rBV	70104	121781	2.39%	0.453%
14	10.628	1274	1282	1289	rBV	1072468	1821273	35.82%	6.775%
15	10.769	1300	1306	1321	rBV	106584	200106	3.94%	0.744%
16	11.281	1388	1393	1402	rBV2	22593	45196	0.89%	0.168%
17	12.163	1538	1543	1545	rVB6	5618	7634	0.15%	0.028%
18	12.651	1621	1626	1629	rBV7	3725	6729	0.13%	0.025%
19	12.787	1646	1649	1653	rVB6	3702	6239	0.12%	0.023%
20	12.840	1653	1658	1662	rVV8	7330	17824	0.35%	0.066%
21	12.887	1664	1666	1672	rVB6	7390	9936	0.20%	0.037%
22	13.357	1743	1746	1752	rBV4	8597	14401	0.28%	0.054%
23	13.451	1758	1762	1765	rVB5	5492	7657	0.15%	0.028%
24	13.875	1827	1834	1842	rBV	195709	280788	5.52%	1.045%
25	13.993	1852	1854	1859	rVB6	7142	7634	0.15%	0.028%
26	14.151	1870	1881	1888	rBV	200830	321070	6.31%	1.194%
27	14.463	1927	1934	1947	rBV	1204284	1843168	36.25%	6.857%
28	15.451	2095	2102	2116	rBV	320656	484042	9.52%	1.801%
29	15.575	2118	2123	2129	rVB2	20893	32450	0.64%	0.121%
30	15.687	2135	2142	2144	rBV7	3726	7704	0.15%	0.029%
31	15.875	2168	2174	2175	rVV6	3110	6159	0.12%	0.023%
32	16.516	2279	2283	2286	rBV5	5203	8666	0.17%	0.032%
33	17.210	2394	2401	2411	rBV	2132380	3097301	60.91%	11.522%
34	17.310	2411	2418	2430	rVB	460079	712402	14.01%	2.650%
35	17.845	2506	2509	2511	rVB2	7244	7191	0.14%	0.027%
36	18.098	2548	2552	2559	rBV3	41826	66795	1.31%	0.248%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018850.D
Acq On : 14 Dec 2023 19:16
Operator : MA/JU
Sample : 05627-19DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD1DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.175	2559	2565	2575	rVV	4232396	5085076	100.00%	18.917%
38	19.198	2735	2739	2744	rBV2	48713	78619	1.55%	0.292%
39	19.251	2744	2748	2751	rVB	46350	56744	1.12%	0.211%
40	19.480	2783	2787	2791	rBV	167887	181133	3.56%	0.674%
41	19.545	2793	2798	2803	rVV	759252	966743	19.01%	3.596%
42	20.498	2957	2960	2964	rBV	120992	123771	2.43%	0.460%
43	21.298	3091	3096	3102	rBV	3137444	3961917	77.91%	14.739%
44	23.498	3465	3470	3476	rBV	505285	911512	17.93%	3.391%
45	23.657	3490	3497	3513	rVB	2248817	4335257	85.25%	16.128%



Sum of corrected areas: 26881097

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018850.D
Acq On : 14 Dec 2023 19:16
Operator : MA/JU
Sample : 05627-19DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

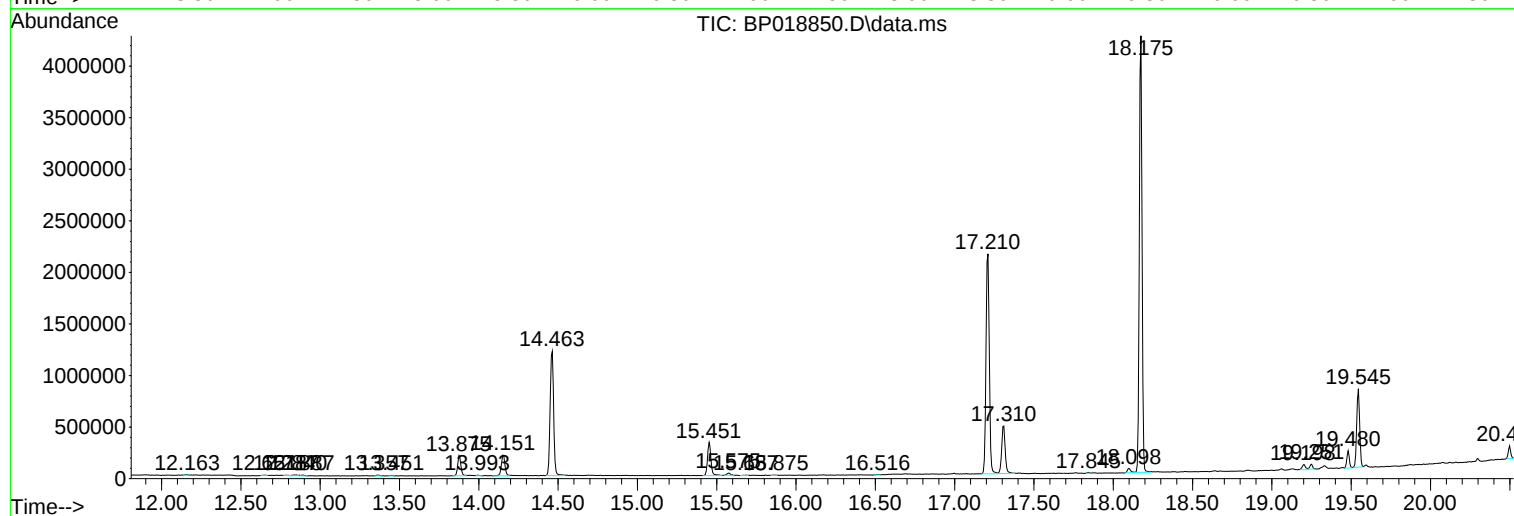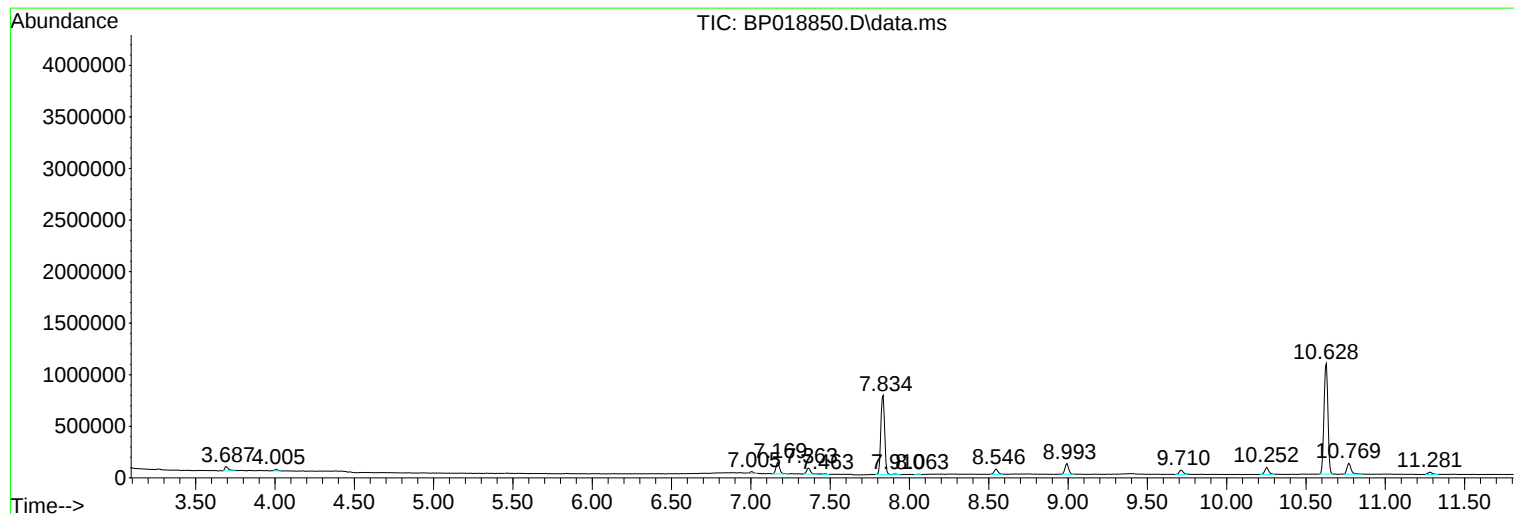

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018850.D
Acq On : 14 Dec 2023 19:16
Operator : MA/JU
Sample : 05627-19DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018850.D
Acq On : 14 Dec 2023 19:16
Operator : MA/JU
Sample : 05627-19DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD1DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc