

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018851.D
 Acq On : 14 Dec 2023 19:50
 Operator : MA/JU
 Sample : 05627-20DL 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	35	rVB5	6759	8350	0.28%	0.044%
2	3.593	84	86	87	rBV2	4748	3511	0.12%	0.018%
3	3.693	99	103	110	rBV3	26659	47624	1.58%	0.248%
4	4.005	154	156	161	rVB2	14719	19042	0.63%	0.099%
5	5.334	377	382	387	rBV5	15128	23699	0.78%	0.124%
6	5.440	398	400	401	rBV2	3755	3420	0.11%	0.018%
7	5.840	463	468	473	rBV7	5397	8939	0.30%	0.047%
8	5.999	491	495	496	rBV4	2616	3196	0.11%	0.017%
9	6.405	562	564	569	rVB5	2577	4145	0.14%	0.022%
10	6.516	576	583	586	rVB9	2769	5746	0.19%	0.030%
11	6.699	612	614	616	rBV3	3233	4083	0.14%	0.021%
12	6.828	632	636	638	rBV5	5292	7514	0.25%	0.039%
13	7.005	662	666	675	rVB3	27863	47700	1.58%	0.249%
14	7.169	689	694	701	rBV	102355	160992	5.33%	0.840%
15	7.363	720	727	733	rBV	84677	138041	4.57%	0.720%
16	7.711	782	786	788	rBV5	2122	3350	0.11%	0.017%
17	7.834	800	807	815	rBV	679032	1085168	35.91%	5.661%
18	7.899	817	818	824	rVB6	5328	7187	0.24%	0.037%
19	8.475	913	916	921	rBV7	1673	3198	0.11%	0.017%
20	8.546	921	928	938	rBV2	64596	128574	4.25%	0.671%
21	8.658	943	947	950	rBV5	2219	3349	0.11%	0.017%
22	8.993	997	1004	1012	rVB	89106	153762	5.09%	0.802%
23	9.246	1044	1047	1049	rBV4	3079	3536	0.12%	0.018%
24	9.328	1058	1061	1064	rBV5	4432	6161	0.20%	0.032%
25	9.716	1120	1127	1134	rBV2	51774	95992	3.18%	0.501%
26	10.157	1198	1202	1206	rBV7	4669	7188	0.24%	0.038%
27	10.252	1210	1218	1226	rBV	94519	172262	5.70%	0.899%
28	10.493	1253	1259	1262	rBV8	3268	5288	0.17%	0.028%
29	10.557	1268	1270	1273	rBV4	2209	3277	0.11%	0.017%
30	10.622	1275	1281	1289	rVB	795594	1363123	45.11%	7.112%
31	10.769	1300	1306	1316	rBV	69648	135561	4.49%	0.707%
32	11.281	1389	1393	1398	rBV7	5281	10410	0.34%	0.054%
33	11.752	1469	1473	1475	rBV5	3105	4980	0.16%	0.026%
34	12.051	1521	1524	1531	rVB9	3542	5875	0.19%	0.031%
35	12.216	1548	1552	1555	rVB6	4243	4706	0.16%	0.025%
36	12.351	1572	1575	1579	rBV6	2760	3641	0.12%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018851.D
 Acq On : 14 Dec 2023 19:50
 Operator : MA/JU
 Sample : 05627-20DL 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	12.404	1582	1584	1585	rBV2	5289	3558	0.12%	0.019%
38	12.681	1629	1631	1635	rVB5	2869	3470	0.11%	0.018%
39	13.004	1683	1686	1689	rVB5	3721	5031	0.17%	0.026%
40	13.204	1718	1720	1723	rBV4	2572	3798	0.13%	0.020%
41	13.310	1731	1738	1743	rBV3	13693	24564	0.81%	0.128%
42	13.363	1743	1747	1748	rBV4	6068	7758	0.26%	0.040%
43	13.740	1808	1811	1814	rBV5	2996	3876	0.13%	0.020%
44	13.875	1827	1834	1841	rBV	206933	308159	10.20%	1.608%
45	13.993	1851	1854	1858	rVB6	6913	10051	0.33%	0.052%
46	14.151	1871	1881	1891	rBV2	212765	383953	12.71%	2.003%
47	14.240	1894	1896	1899	rVB4	4204	4148	0.14%	0.022%
48	14.463	1927	1934	1946	rBV	1098687	1687871	55.85%	8.806%
49	14.687	1967	1972	1973	rBV5	7630	8576	0.28%	0.045%
50	14.881	2003	2005	2007	rBV3	3663	4304	0.14%	0.022%
51	14.922	2009	2012	2016	rBV6	2753	4097	0.14%	0.021%
52	15.451	2096	2102	2112	rBV	346433	509774	16.87%	2.660%
53	15.575	2118	2123	2130	rVB2	38874	63887	2.11%	0.333%
54	15.687	2139	2142	2146	rBV6	3227	5269	0.17%	0.027%
55	15.857	2168	2171	2176	rBV7	4886	7754	0.26%	0.040%
56	16.963	2357	2359	2361	rBV3	4010	3482	0.12%	0.018%
57	17.210	2394	2401	2411	rBV	1430542	2130264	70.49%	11.114%
58	17.304	2411	2417	2427	rVV2	360808	551550	18.25%	2.877%
59	17.763	2490	2495	2498	rBV7	6379	13036	0.43%	0.068%
60	18.098	2548	2552	2557	rBV2	54800	70827	2.34%	0.370%
61	18.169	2559	2564	2572	rVV	1988592	2437226	80.65%	12.715%
62	19.204	2736	2740	2750	rBV5	21305	48113	1.59%	0.251%
63	19.333	2759	2762	2766	rVB4	23431	27535	0.91%	0.144%
64	19.545	2793	2798	2804	rBV	565850	774639	25.63%	4.041%
65	21.298	3091	3096	3103	rBV	1872622	2483224	82.17%	12.955%
66	23.498	3466	3470	3485	rVB2	422800	863286	28.57%	4.504%
67	23.657	3490	3497	3506	rVB	1514754	3022053	100.00%	15.766%




Sum of corrected areas: 19167723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018851.D
Acq On : 14 Dec 2023 19:50
Operator : MA/JU
Sample : 05627-20DL 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

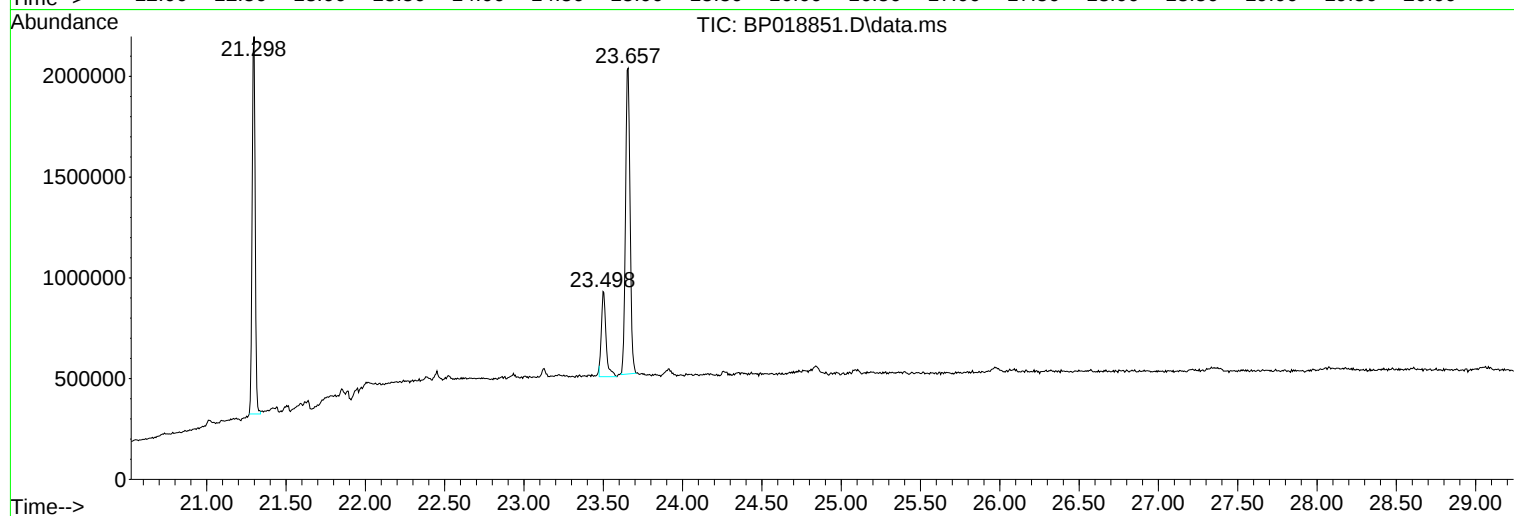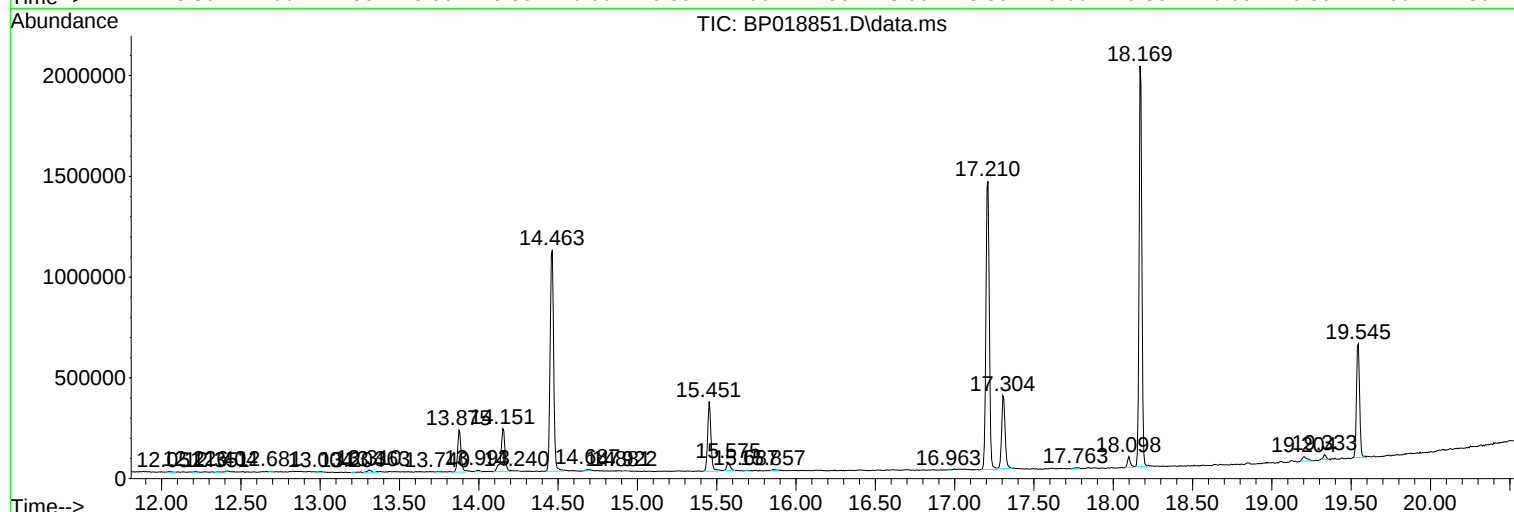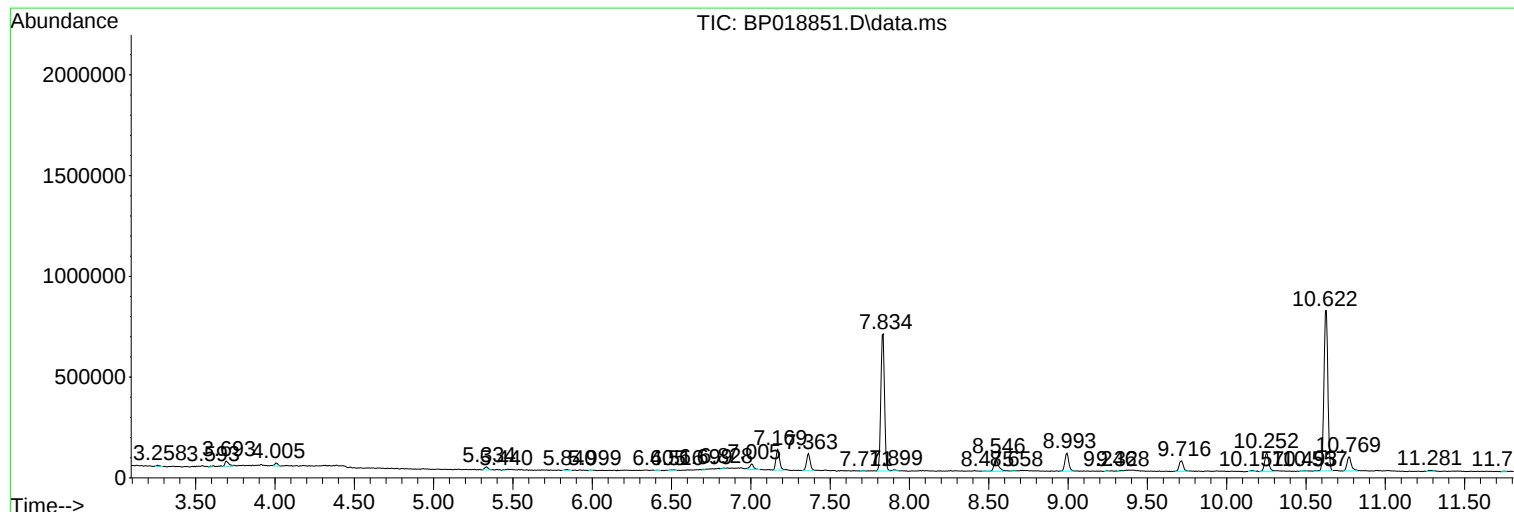

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018851.D
Acq On : 14 Dec 2023 19:50
Operator : MA/JU
Sample : 05627-20DL 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018851.D
Acq On : 14 Dec 2023 19:50
Operator : MA/JU
Sample : 05627-20DL 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc