

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018852.D
 Acq On : 14 Dec 2023 20:24
 Operator : MA/JU
 Sample : 05627-18DL 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	32	rVB4	7300	8820	0.16%	0.032%
2	3.693	99	103	109	rBV	29064	49267	0.88%	0.178%
3	4.005	153	156	160	rVB2	14771	16982	0.30%	0.061%
4	5.334	378	382	386	rBV2	8626	11923	0.21%	0.043%
5	5.469	399	405	408	rBV2	21665	38811	0.69%	0.140%
6	5.834	463	467	473	rVB4	13924	22065	0.39%	0.080%
7	6.234	533	535	539	rBV5	4471	6596	0.12%	0.024%
8	6.922	648	652	655	rBV6	4940	7309	0.13%	0.026%
9	7.005	661	666	673	rVB	27268	45197	0.81%	0.164%
10	7.169	689	694	703	rBV	128038	199188	3.56%	0.721%
11	7.363	720	727	734	rBV	106510	173750	3.11%	0.629%
12	7.475	743	746	750	rVB6	3904	5592	0.10%	0.020%
13	7.834	800	807	815	rBV	876563	1429656	25.59%	5.172%
14	7.904	815	819	821	rVV5	4827	5791	0.10%	0.021%
15	8.546	921	928	937	rBV3	70259	134203	2.40%	0.486%
16	8.646	943	945	952	rVB6	6799	11145	0.20%	0.040%
17	8.922	989	992	995	rVB4	6077	6619	0.12%	0.024%
18	8.993	997	1004	1009	rBV	119663	199486	3.57%	0.722%
19	9.546	1093	1098	1104	rVB10	5229	11779	0.21%	0.043%
20	9.710	1120	1126	1133	rBV	70978	119431	2.14%	0.432%
21	10.251	1211	1218	1228	rBV	122622	222536	3.98%	0.805%
22	10.628	1274	1282	1289	rVB	1032592	1781811	31.89%	6.446%
23	10.769	1300	1306	1321	rBV	102149	198815	3.56%	0.719%
24	11.287	1385	1394	1399	rVB9	6627	16900	0.30%	0.061%
25	11.828	1483	1486	1489	rBV4	4677	6799	0.12%	0.025%
26	11.898	1491	1498	1500	rVV6	5405	10546	0.19%	0.038%
27	12.404	1578	1584	1596	rBV	33408	69600	1.25%	0.252%
28	13.251	1723	1728	1731	rBV7	2787	5878	0.11%	0.021%
29	13.369	1742	1748	1752	rBV7	9651	15413	0.28%	0.056%
30	13.875	1828	1834	1841	rBV	265790	377598	6.76%	1.366%
31	14.151	1875	1881	1892	rBV	263476	417157	7.47%	1.509%
32	14.298	1904	1906	1911	rVB6	5993	6229	0.11%	0.023%
33	14.381	1914	1920	1921	rBV6	5359	8273	0.15%	0.030%
34	14.457	1927	1933	1943	rVB	1245166	1917694	34.32%	6.938%
35	14.686	1967	1972	1974	rBV6	7531	12530	0.22%	0.045%
36	14.869	1998	2003	2008	rBV9	4384	8246	0.15%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018852.D
 Acq On : 14 Dec 2023 20:24
 Operator : MA/JU
 Sample : 05627-18DL 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.051	2023	2034	2035	rBV6	4854	13532	0.24%	0.049%
38	15.451	2096	2102	2114	rBV	428766	636368	11.39%	2.302%
39	15.575	2118	2123	2132	rVB2	49014	81702	1.46%	0.296%
40	17.016	2365	2368	2374	rBV	17300	24031	0.43%	0.087%
41	17.210	2394	2401	2412	rBV	1752705	2574461	46.07%	9.314%
42	17.304	2412	2417	2428	rVB2	463491	680384	12.18%	2.461%
43	17.551	2458	2459	2463	rBV3	4768	6229	0.11%	0.023%
44	17.839	2506	2508	2512	rVB	6115	5931	0.11%	0.021%
45	18.098	2548	2552	2559	rBV2	59879	89076	1.59%	0.322%
46	18.175	2559	2565	2572	rBV	4780261	5587861	100.00%	20.215%
47	19.333	2758	2762	2766	rBV4	44495	53620	0.96%	0.194%
48	19.545	2793	2798	2805	rBV	727777	960864	17.20%	3.476%
49	21.298	3091	3096	3105	rBV	2795397	3537840	63.31%	12.799%
50	21.851	3187	3190	3196	rVB2	138638	173884	3.11%	0.629%
51	22.451	3288	3292	3299	rVB	222879	340549	6.09%	1.232%
52	23.127	3403	3407	3414	rVB	247316	420284	7.52%	1.520%
53	23.498	3465	3470	3476	rBV	522868	975427	17.46%	3.529%
54	23.657	3490	3497	3509	rVB	1966668	3899901	69.79%	14.109%




Sum of corrected areas: 27641579

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018852.D
Acq On : 14 Dec 2023 20:24
Operator : MA/JU
Sample : 05627-18DL 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

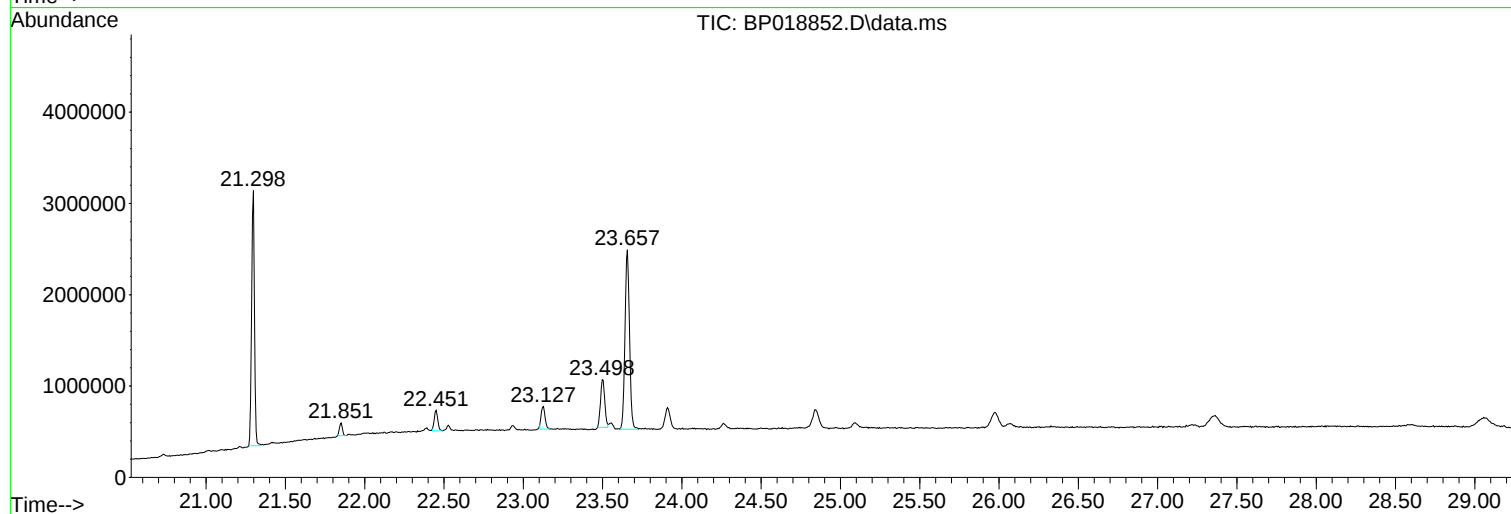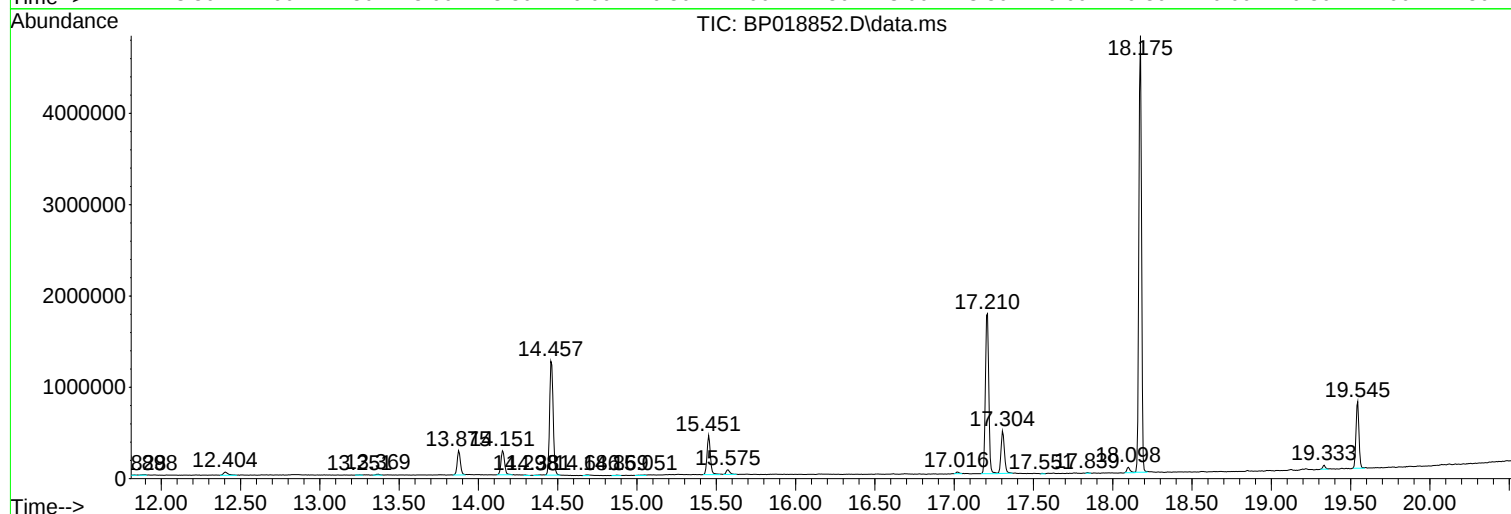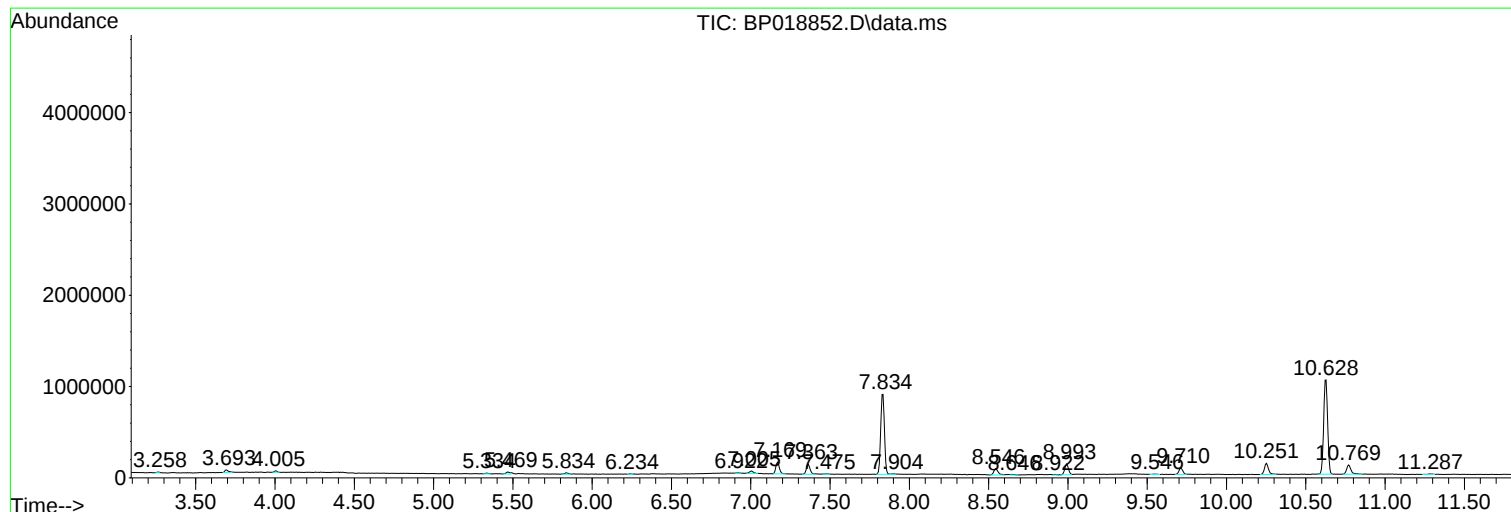

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018852.D
Acq On : 14 Dec 2023 20:24
Operator : MA/JU
Sample : 05627-18DL 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
DCLD0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexasiloxane, tetradecamethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
23.127	2.16 ng/ul	420284	Perylene-d12	23.657	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	68
2	Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	49
3	Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	40
4	Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	38
5	3-Isopropoxy-1,1,1,7,7,7-hexamet...	576	C18H52O7Si7	071579-69-6	27

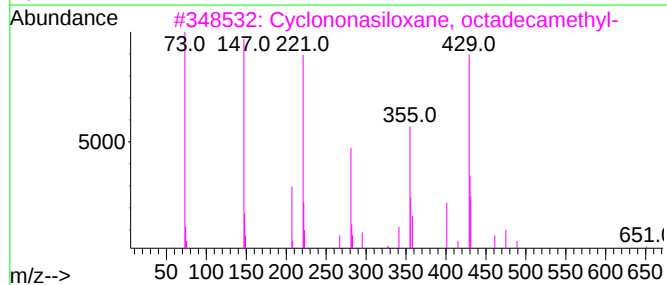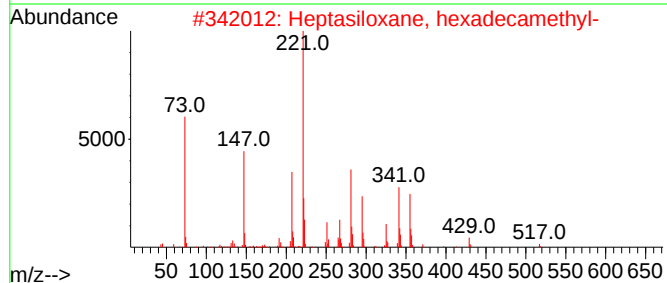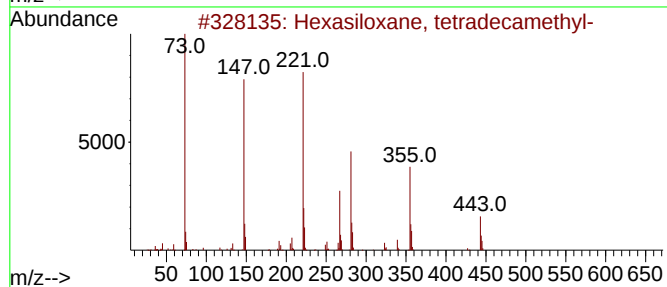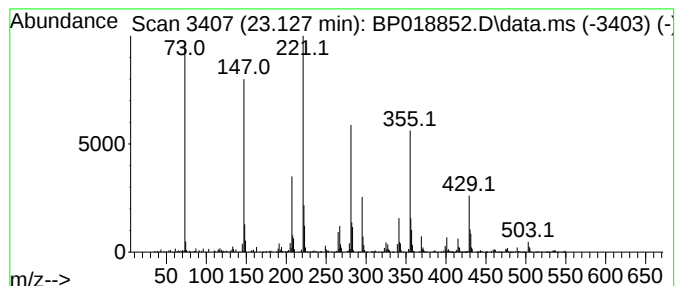

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018852.D
Acq On : 14 Dec 2023 20:24
Operator : MA/JU
Sample : 05627-18DL 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexasiloxane, t...	23.127	2.2	ng/u1	420284	6	23.657	3899900	20.0