

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018855.D
 Acq On : 14 Dec 2023 22:06
 Operator : MA/JU
 Sample : 05627-21DL 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	36	rVB2	16965	23587	0.56%	0.077%
2	3.687	99	102	113	rBV	50770	86033	2.04%	0.281%
3	4.005	154	156	161	rVB	18962	22128	0.52%	0.072%
4	5.287	370	374	375	rBV4	3113	4472	0.11%	0.015%
5	5.334	379	382	386	rVB5	7139	8623	0.20%	0.028%
6	5.469	401	405	408	rBV	7999	12123	0.29%	0.040%
7	5.693	437	443	445	rVV7	2799	5083	0.12%	0.017%
8	5.840	464	468	472	rBV4	7247	10334	0.24%	0.034%
9	6.328	546	551	553	rBV6	2968	5054	0.12%	0.016%
10	6.511	578	582	588	rVB4	18245	29981	0.71%	0.098%
11	6.822	633	635	643	rVB4	9480	16673	0.39%	0.054%
12	7.005	661	666	671	rVB	59803	94576	2.24%	0.309%
13	7.169	688	694	702	rBV	247838	378409	8.96%	1.235%
14	7.364	721	727	733	rBV	218406	347378	8.22%	1.134%
15	7.828	799	806	815	rBV	994259	1583248	37.47%	5.167%
16	7.899	815	818	827	rVV3	15034	28577	0.68%	0.093%
17	8.405	900	904	910	rBV7	8127	16121	0.38%	0.053%
18	8.540	922	927	937	rBV	133044	236430	5.60%	0.772%
19	8.993	998	1004	1012	rVV	226419	373867	8.85%	1.220%
20	9.163	1027	1033	1037	rVB7	6185	8457	0.20%	0.028%
21	9.710	1117	1126	1133	rBV	144948	246536	5.83%	0.805%
22	9.852	1145	1150	1151	rBV4	3523	4352	0.10%	0.014%
23	9.946	1162	1166	1174	rVB8	10566	17614	0.42%	0.057%
24	10.040	1179	1182	1186	rBV5	4057	5494	0.13%	0.018%
25	10.163	1198	1203	1206	rBV7	4712	9096	0.22%	0.030%
26	10.246	1211	1217	1228	rBV	246228	430546	10.19%	1.405%
27	10.405	1243	1244	1249	rVB5	3431	4561	0.11%	0.015%
28	10.487	1256	1258	1262	rVB5	5865	7577	0.18%	0.025%
29	10.622	1274	1281	1289	rBV	1185317	1980765	46.88%	6.464%
30	10.681	1289	1291	1299	rVB8	6714	10313	0.24%	0.034%
31	10.769	1299	1306	1319	rBV	233427	414549	9.81%	1.353%
32	11.134	1365	1368	1372	rBV6	3501	4723	0.11%	0.015%
33	11.281	1389	1393	1396	rBV4	7838	12511	0.30%	0.041%
34	11.422	1413	1417	1428	rVB4	8715	17773	0.42%	0.058%
35	11.893	1491	1497	1499	rBV5	4570	5995	0.14%	0.020%
36	12.210	1547	1551	1557	rVB7	5609	9775	0.23%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018855.D
 Acq On : 14 Dec 2023 22:06
 Operator : MA/JU
 Sample : 05627-21DL 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	12.404	1579	1584	1591	rBV2	16835	35731	0.85%	0.117%
38	13.081	1698	1699	1705	rVB6	3168	4709	0.11%	0.015%
39	13.216	1719	1722	1724	rBV4	3493	4271	0.10%	0.014%
40	13.293	1732	1735	1737	rBV4	4648	6050	0.14%	0.020%
41	13.369	1742	1748	1751	rBV5	8988	15784	0.37%	0.052%
42	13.604	1785	1788	1792	rVB6	3664	4954	0.12%	0.016%
43	13.875	1823	1834	1841	rBV	486988	695169	16.45%	2.269%
44	14.151	1871	1881	1895	rBV	540335	805125	19.06%	2.627%
45	14.463	1926	1934	1945	rBV	1505697	2315073	54.79%	7.555%
46	14.675	1966	1970	1982	rVB5	20332	48368	1.14%	0.158%
47	15.210	2056	2061	2063	rVB6	3554	4947	0.12%	0.016%
48	15.404	2090	2094	2096	rBV4	3288	4237	0.10%	0.014%
49	15.451	2096	2102	2116	rVV	668300	1003594	23.75%	3.275%
50	15.569	2116	2122	2133	rBV	105904	176937	4.19%	0.577%
51	15.863	2168	2172	2179	rVB10	7082	10864	0.26%	0.035%
52	15.928	2181	2183	2188	rVB6	3902	6185	0.15%	0.020%
53	16.410	2261	2265	2268	rBV6	3547	5142	0.12%	0.017%
54	16.510	2280	2282	2286	rBV5	3810	5440	0.13%	0.018%
55	16.639	2302	2304	2307	rBV3	4037	4462	0.11%	0.015%
56	17.022	2365	2369	2373	rBV3	10661	16754	0.40%	0.055%
57	17.210	2394	2401	2411	rBV	1870225	2807318	66.44%	9.162%
58	17.304	2411	2417	2428	rVV	888164	1258373	29.78%	4.107%
59	18.098	2548	2552	2557	rBV3	56473	80536	1.91%	0.263%
60	18.169	2559	2564	2576	rVB	2397797	2903358	68.71%	9.475%
61	19.192	2735	2738	2740	rBV3	18413	21809	0.52%	0.071%
62	19.545	2792	2798	2804	rBV	1360427	1817454	43.01%	5.931%
63	21.298	3091	3096	3105	rBV	3001055	3763364	89.07%	12.282%
64	23.498	3465	3470	3485	rVB2	1081842	2117706	50.12%	6.911%
65	23.657	3490	3497	3509	rVB	2113127	4225266	100.00%	13.789%




Sum of corrected areas: 30642314

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018855.D
Acq On : 14 Dec 2023 22:06
Operator : MA/JU
Sample : 05627-21DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

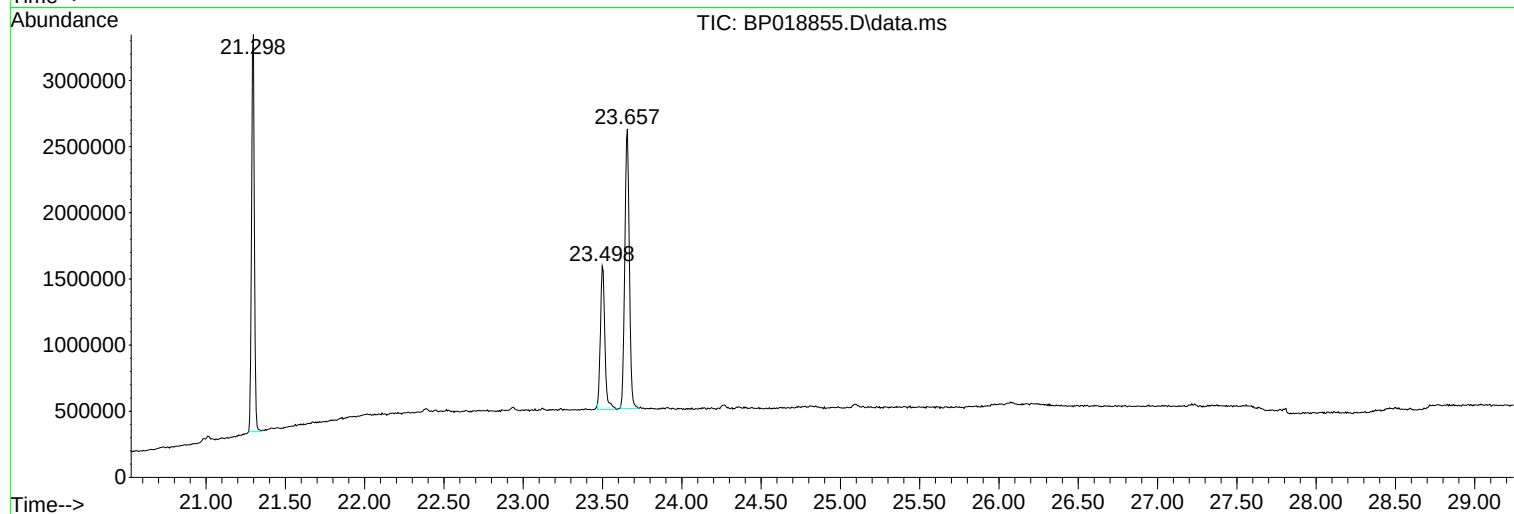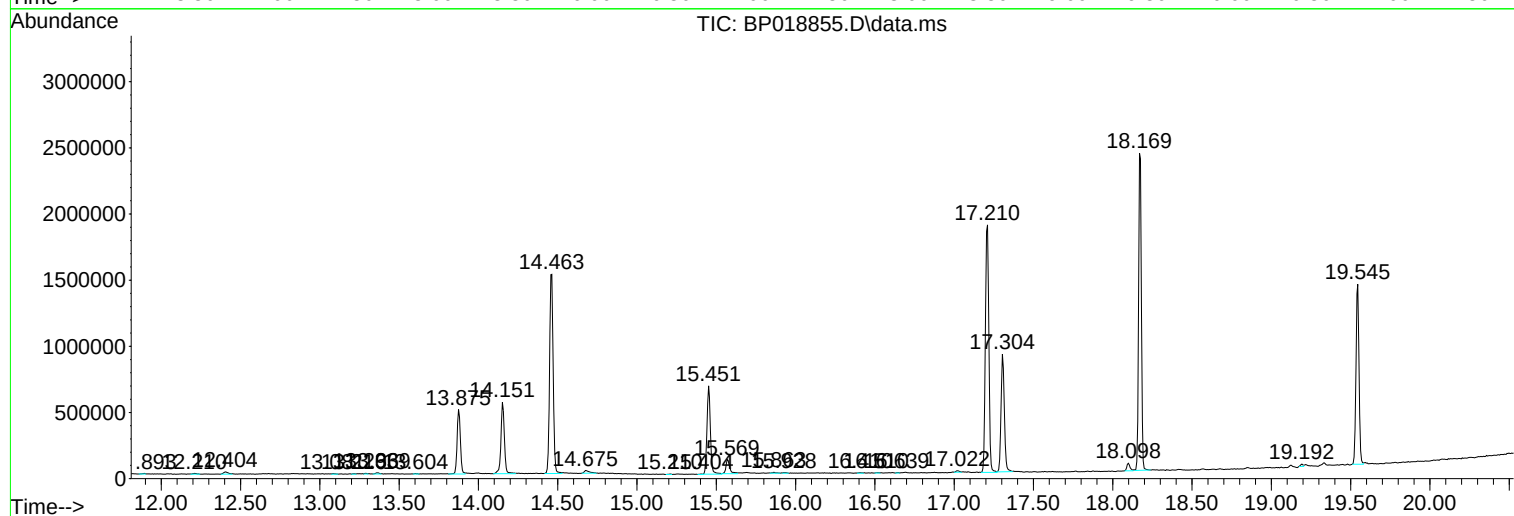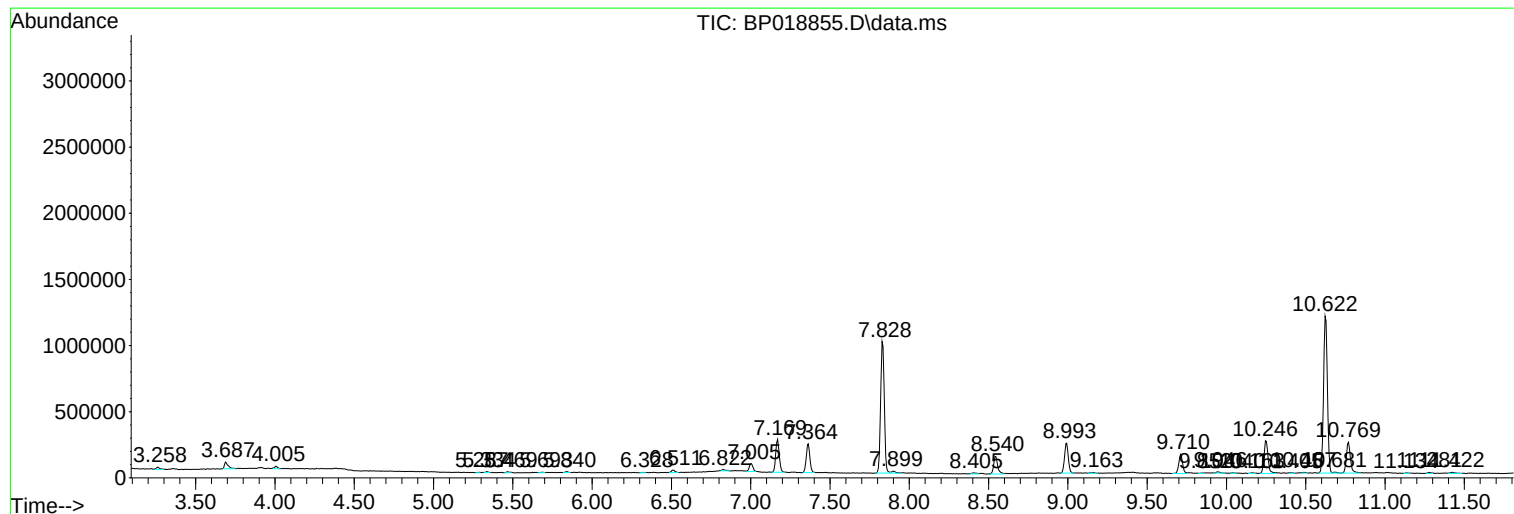

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018855.D
Acq On : 14 Dec 2023 22:06
Operator : MA/JU
Sample : 05627-21DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018855.D
Acq On : 14 Dec 2023 22:06
Operator : MA/JU
Sample : 05627-21DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc