

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018866.D
 Acq On : 15 Dec 2023 04:52
 Operator : MA/JU
 Sample : PB157755BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK755

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	35	rBV	90516	117491	1.41%	0.175%
2	3.675	96	100	118	rBV	1064228	1626222	19.48%	2.420%
3	4.005	153	156	160	rVB2	18519	24071	0.29%	0.036%
4	4.334	209	212	217	rBV3	17473	22856	0.27%	0.034%
5	6.999	659	665	676	rVB	1150746	1815850	21.76%	2.702%
6	7.169	684	694	702	rVB	1004090	1518098	18.19%	2.259%
7	7.358	719	726	735	rBV	1179174	1874600	22.46%	2.790%
8	7.828	798	806	814	rBV	919316	1445815	17.32%	2.152%
9	8.540	920	927	942	rBV	1415379	2284319	27.37%	3.399%
10	8.993	997	1004	1017	rBV	1071327	1709569	20.48%	2.544%
11	9.710	1117	1126	1144	rBV	821785	1354471	16.23%	2.016%
12	10.246	1207	1217	1232	rBV	1387668	2301330	27.57%	3.425%
13	10.622	1274	1281	1289	rVB	1145122	1829754	21.92%	2.723%
14	10.763	1298	1305	1318	rBV	1370493	2349624	28.15%	3.497%
15	11.893	1491	1497	1504	rVB	5706	12976	0.16%	0.019%
16	12.210	1545	1551	1557	rBV2	25433	41817	0.50%	0.062%
17	13.363	1738	1747	1752	rBV3	21345	36695	0.44%	0.055%
18	13.434	1754	1759	1763	rBV7	4649	8973	0.11%	0.013%
19	13.875	1827	1834	1845	rBV	2328932	3234882	38.76%	4.814%
20	14.151	1873	1881	1896	rBV	2593667	3857070	46.21%	5.740%
21	14.463	1927	1934	1945	rBV	1457644	2213361	26.52%	3.294%
22	14.663	1962	1968	1989	rBV	844770	1476557	17.69%	2.197%
23	15.451	2096	2102	2116	rBV	3336567	4866441	58.31%	7.242%
24	15.575	2116	2123	2134	rVV	808857	1127517	13.51%	1.678%
25	15.693	2139	2143	2152	rVB3	20565	35754	0.43%	0.053%
26	16.892	2343	2347	2351	rBV7	6728	10468	0.13%	0.016%
27	16.992	2362	2364	2372	rBV6	6140	12373	0.15%	0.018%
28	17.210	2394	2401	2408	rBV	1701304	2483917	29.76%	3.696%
29	17.310	2411	2418	2435	rVV	3682779	5403676	64.74%	8.042%
30	17.763	2491	2495	2501	rVB6	5708	9848	0.12%	0.015%
31	18.098	2549	2552	2556	rBV6	16674	22646	0.27%	0.034%
32	19.122	2722	2726	2733	rVB	52203	68165	0.82%	0.101%
33	19.186	2734	2737	2742	rVV	46188	59689	0.72%	0.089%
34	19.545	2792	2798	2806	rBV	5302773	6817037	81.68%	10.145%
35	21.298	3091	3096	3105	rBV	2536963	3198671	38.32%	4.760%
36	23.510	3464	3472	3487	rVB	4179562	8346175	100.00%	12.421%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018866.D
Acq On : 15 Dec 2023 04:52
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.657	3491	3497	3510	rVB	1776820	3577764	42.87%	5.324%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 67196542

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018866.D
Acq On : 15 Dec 2023 04:52
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

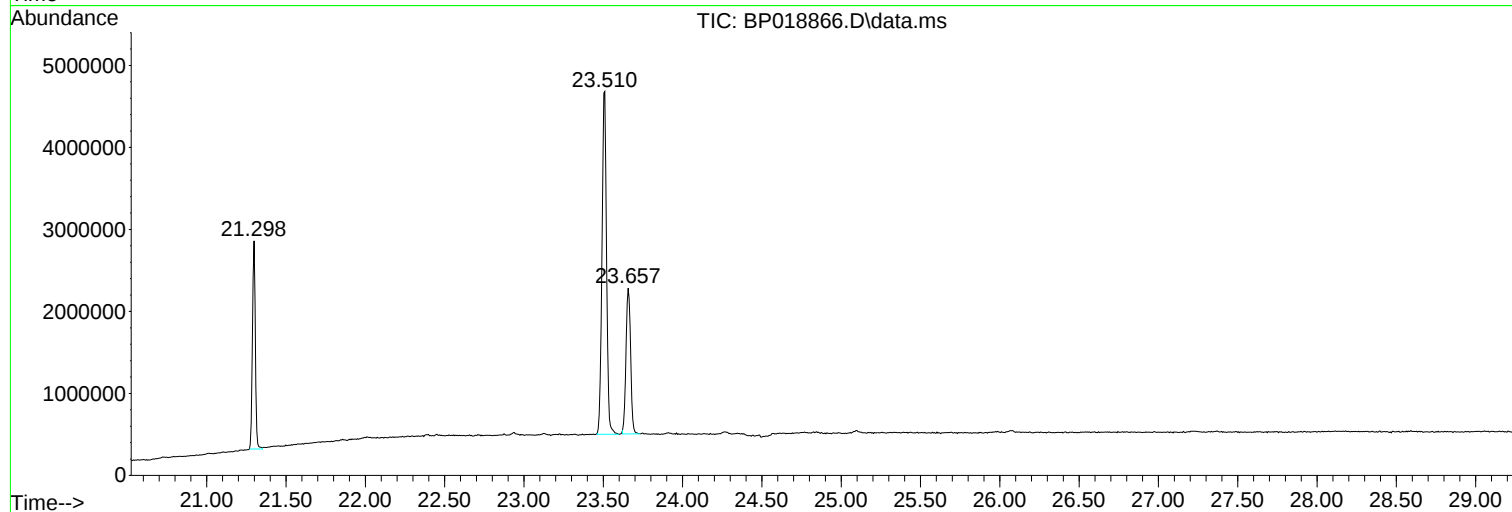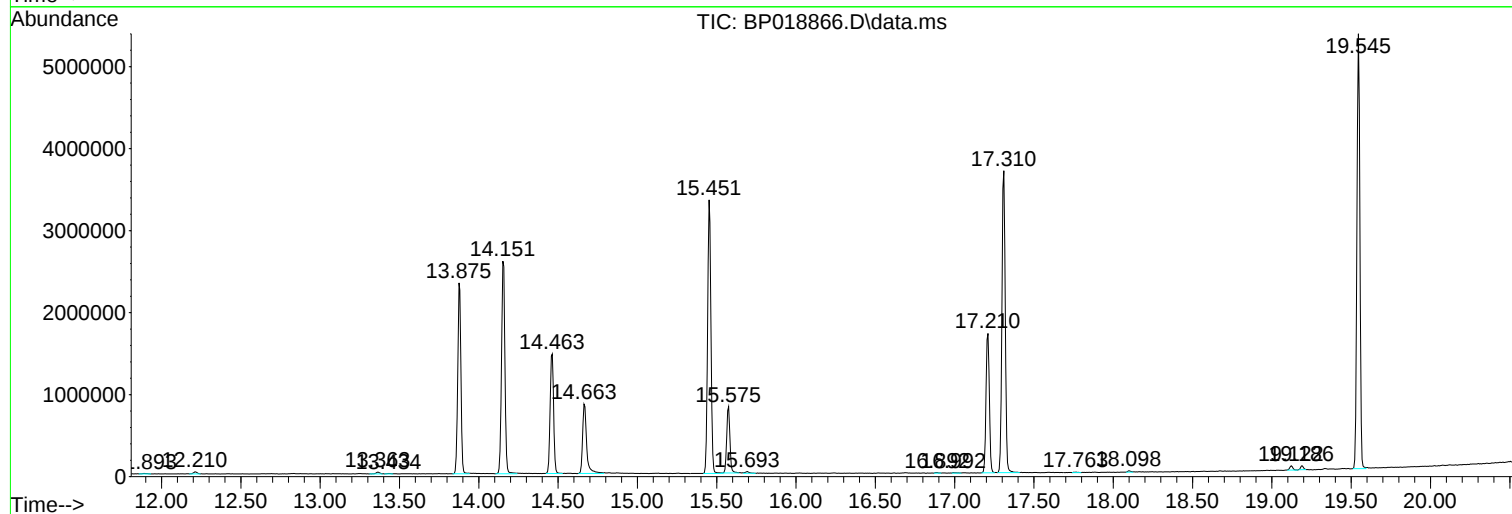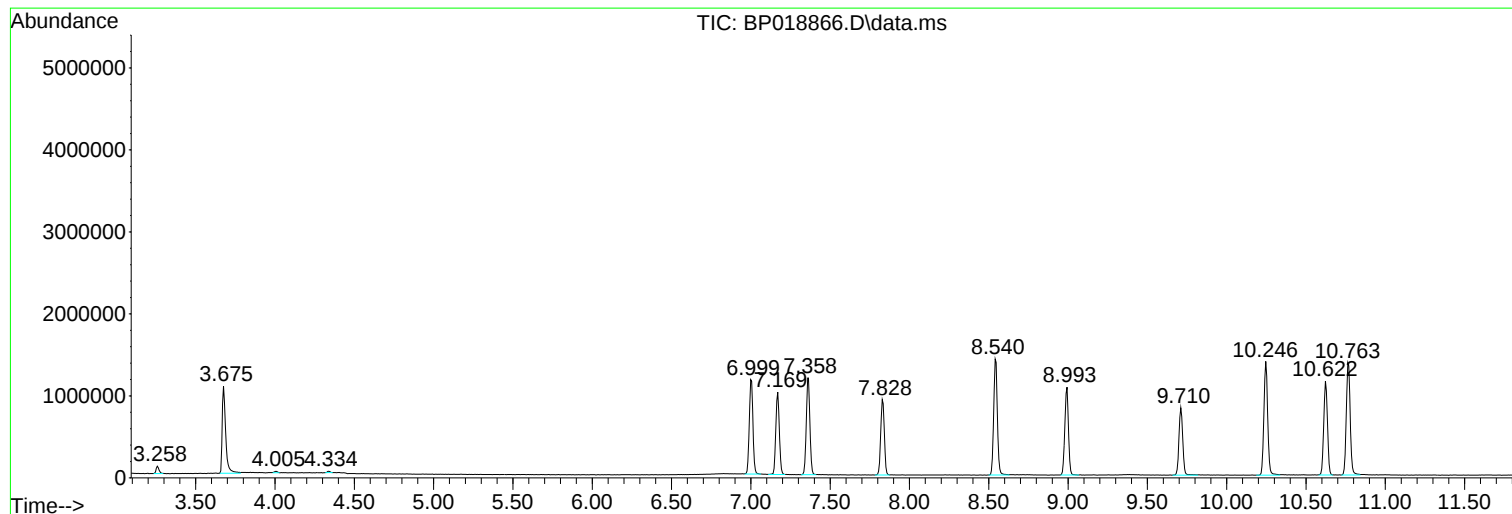

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018866.D
Acq On : 15 Dec 2023 04:52
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018866.D
Acq On : 15 Dec 2023 04:52
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc