

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
 Data File : BP018867.D
 Acq On : 15 Dec 2023 05:26
 Operator : MA/JU
 Sample : PB157687BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	37	rVB	90265	113294	1.79%	0.202%
2	3.675	96	100	117	rBV	952871	1430203	22.63%	2.547%
3	4.005	152	156	161	rVB	20403	30068	0.48%	0.054%
4	6.999	659	665	676	rVB	1057759	1613692	25.54%	2.874%
5	7.169	687	694	702	rVB	868592	1341218	21.23%	2.388%
6	7.357	719	726	735	rVB	1077576	1670387	26.44%	2.975%
7	7.828	799	806	817	rVB	915065	1431216	22.65%	2.549%
8	8.052	842	844	849	rVB6	5797	9717	0.15%	0.017%
9	8.540	916	927	942	rBV	1213189	1962495	31.06%	3.495%
10	8.993	996	1004	1014	rBV	895899	1483057	23.47%	2.641%
11	9.710	1118	1126	1136	rBV	707859	1116400	17.67%	1.988%
12	10.246	1205	1217	1232	rBV	1159631	1925183	30.47%	3.428%
13	10.481	1253	1257	1260	rBV6	3682	7191	0.11%	0.013%
14	10.622	1272	1281	1290	rVB	1119208	1851161	29.30%	3.297%
15	10.763	1298	1305	1318	rBV	1085178	1868331	29.57%	3.327%
16	11.881	1493	1495	1505	rVB10	5144	12952	0.20%	0.023%
17	12.210	1545	1551	1560	rVB	21268	41112	0.65%	0.073%
18	13.245	1722	1727	1731	rBV7	4162	8575	0.14%	0.015%
19	13.357	1743	1746	1755	rVB6	15157	26404	0.42%	0.047%
20	13.440	1755	1760	1764	rBV8	4673	9229	0.15%	0.016%
21	13.598	1783	1787	1792	rBV6	3785	7886	0.12%	0.014%
22	13.875	1827	1834	1843	rBV	1399954	2050440	32.45%	3.651%
23	14.051	1862	1864	1870	rVB5	7654	11171	0.18%	0.020%
24	14.151	1870	1881	1893	rBV	1798684	2659726	42.09%	4.736%
25	14.457	1926	1933	1942	rBV	1512884	2207867	34.94%	3.932%
26	14.663	1962	1968	1992	rBV	600077	1080788	17.10%	1.925%
27	15.257	2063	2069	2072	rBV8	5556	10251	0.16%	0.018%
28	15.451	2096	2102	2116	rBV	2682751	3771137	59.68%	6.716%
29	15.575	2116	2123	2132	rBV	508793	725234	11.48%	1.292%
30	15.692	2139	2143	2148	rVB6	14372	22262	0.35%	0.040%
31	16.992	2362	2364	2368	rVB5	6023	7097	0.11%	0.013%
32	17.210	2394	2401	2410	rBV	1857957	2587317	40.95%	4.608%
33	17.304	2411	2417	2429	rVV	2753353	4014323	63.53%	7.149%
34	18.098	2549	2552	2555	rBV5	18087	24781	0.39%	0.044%
35	19.122	2722	2726	2732	rVB2	44409	57690	0.91%	0.103%
36	19.192	2734	2738	2742	rVV	36218	47450	0.75%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018867.D
Acq On : 15 Dec 2023 05:26
Operator : MA/JU
Sample : PB157687BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.333	2759	2762	2766	rBV5	16374	24617	0.39%	0.044%
38	19.545	2792	2798	2805	rBV	4119426	5284518	83.63%	9.411%
39	21.298	3091	3096	3104	rBV	2779745	3449039	54.58%	6.142%
40	23.504	3464	3471	3485	rVB2	3130470	6318743	100.00%	11.253%
41	23.657	3490	3497	3510	rVB	1855831	3839677	60.77%	6.838%




Sum of corrected areas: 56153899

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018867.D
Acq On : 15 Dec 2023 05:26
Operator : MA/JU
Sample : PB157687BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

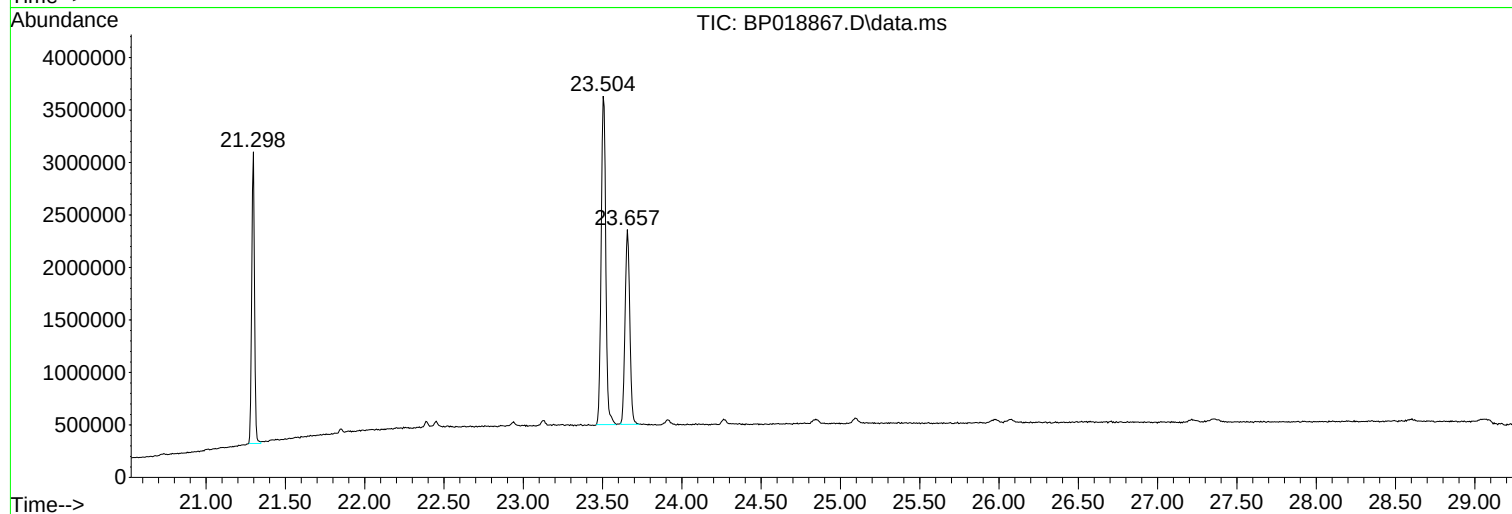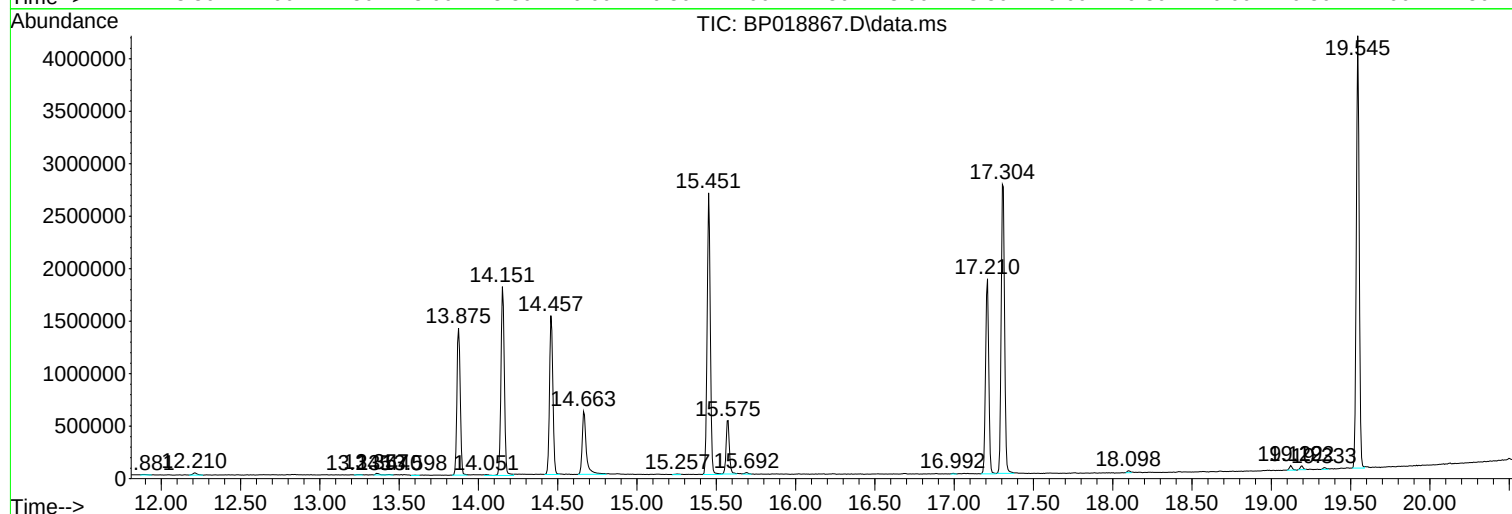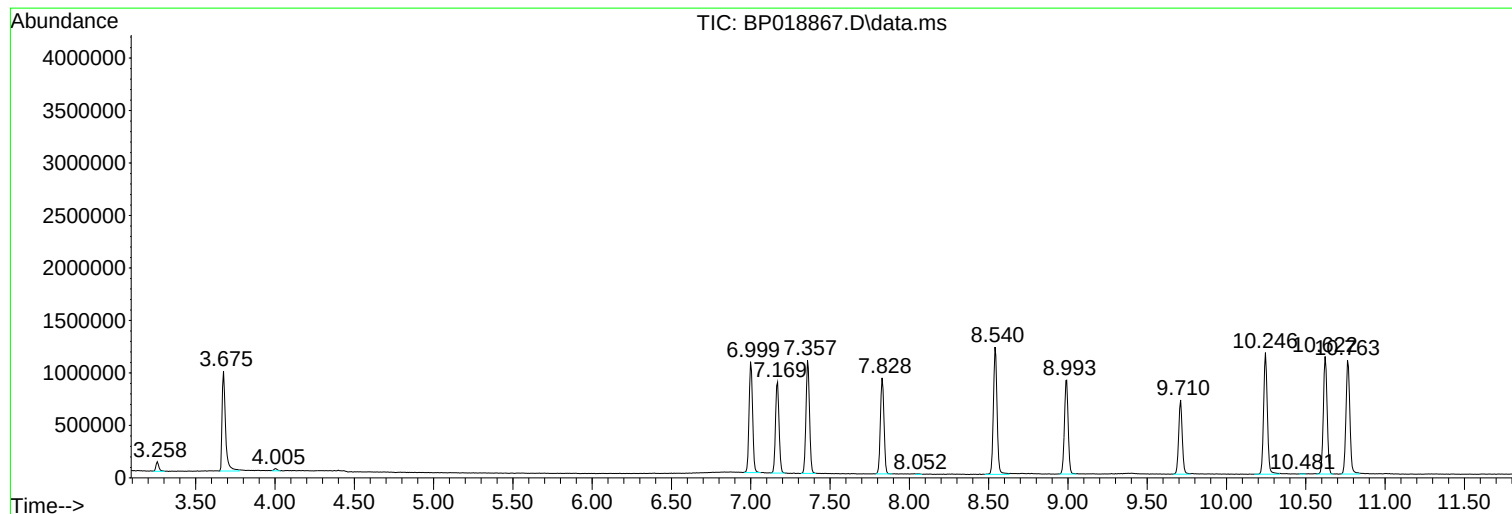

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018867.D
Acq On : 15 Dec 2023 05:26
Operator : MA/JU
Sample : PB157687BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121323\
Data File : BP018867.D
Acq On : 15 Dec 2023 05:26
Operator : MA/JU
Sample : PB157687BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------