
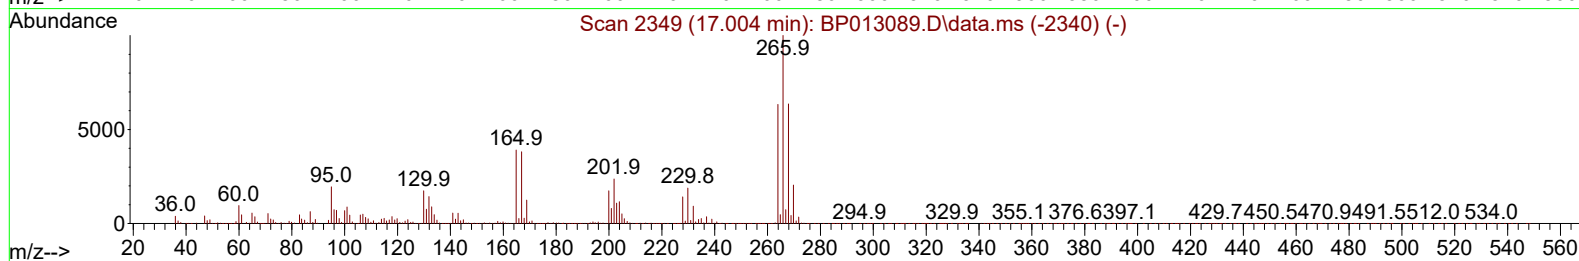
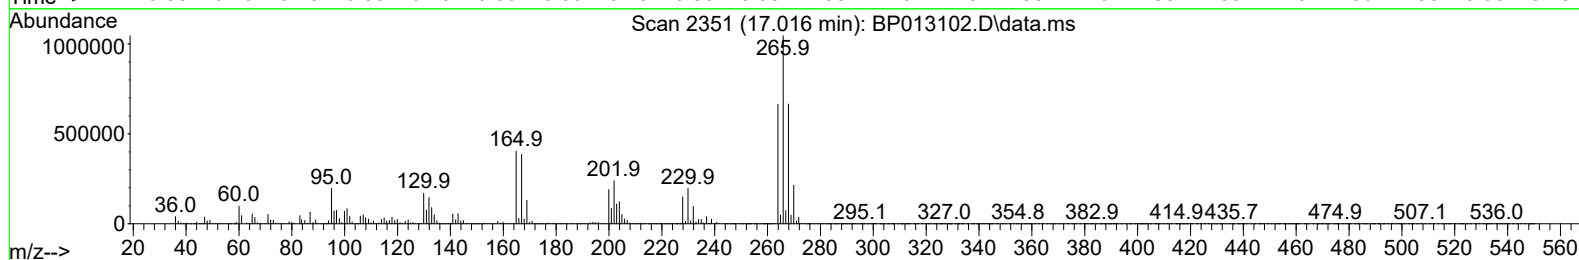


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121422\
Data File : BP013102.D
Acq On : 14 Dec 2022 10:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:18:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

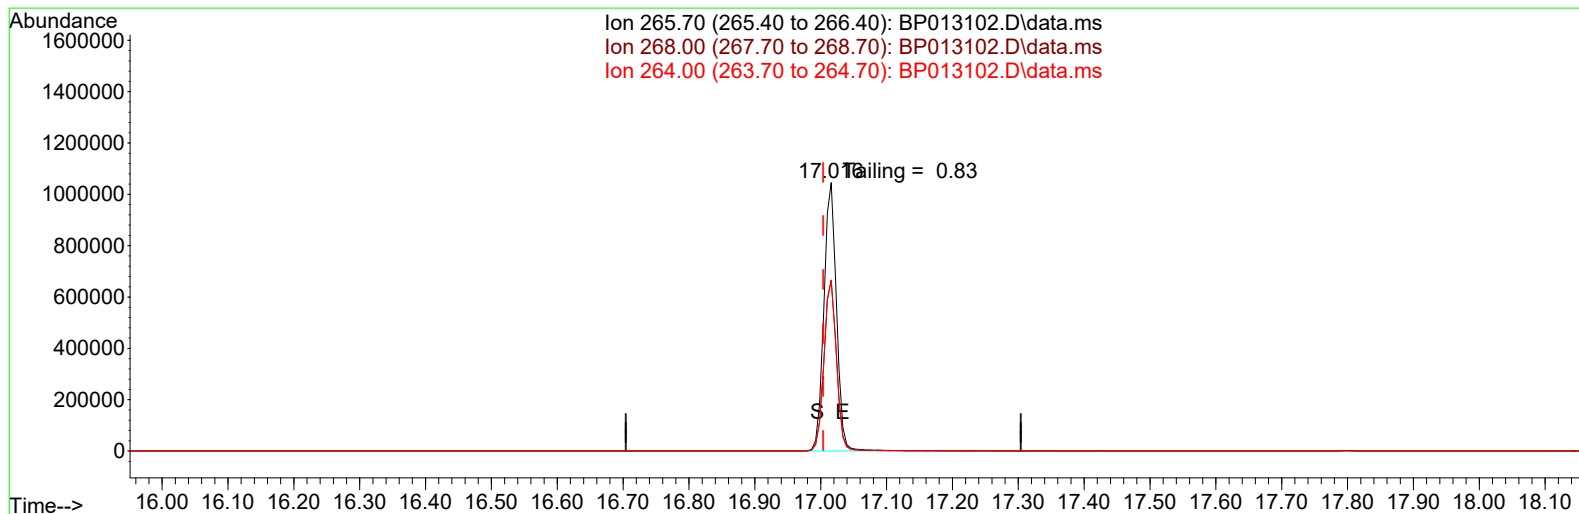

TIC: BP013102.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.012) 35617.47 ng

response 1386707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.66
264.00	63.30	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121422\
 Data File : BP013102.D
 Acq On : 14 Dec 2022 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 05:18:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

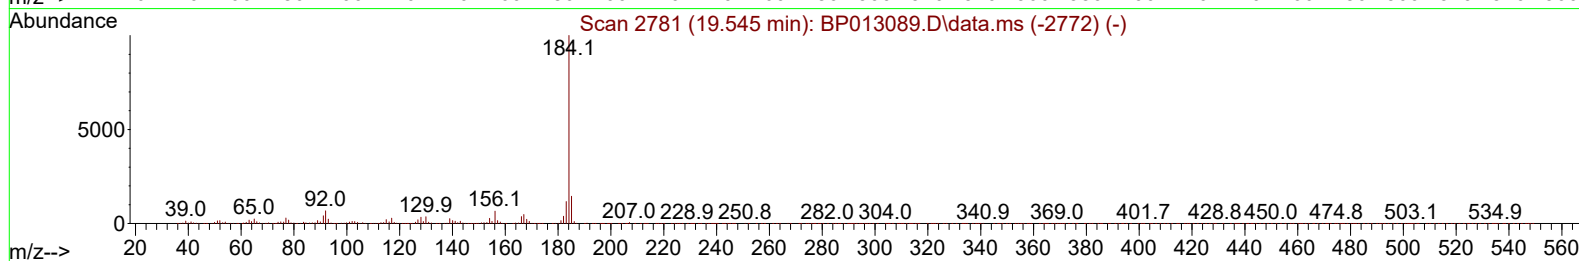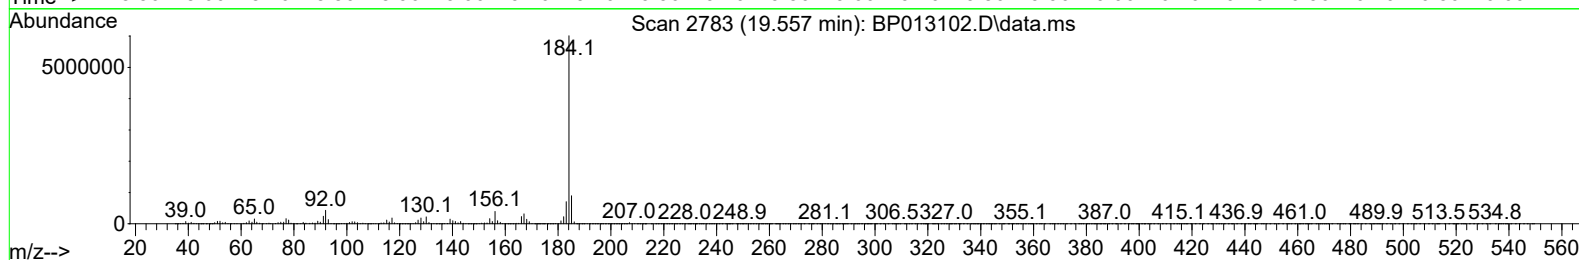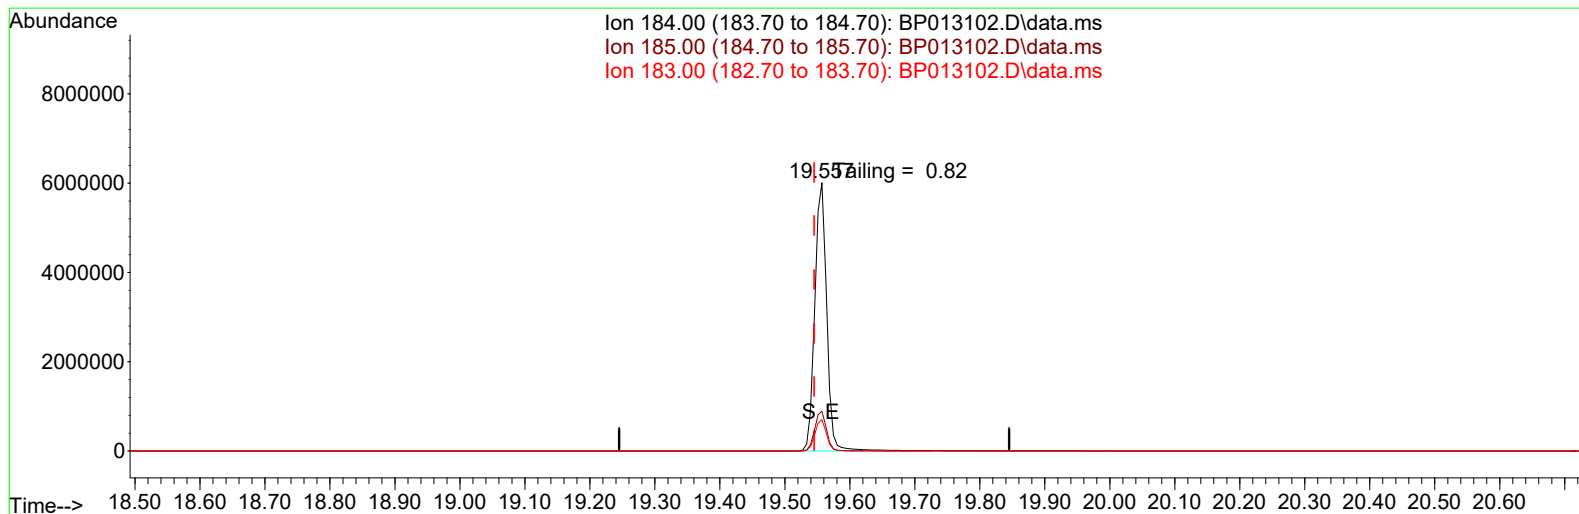

TIC: BP013102.D\data.ms

(77) Benzidine

19.557min (+ 0.012) 24878.84 ng

response 7670848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.87
183.00	11.70	11.73
0.00	0.00	0.00