


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121422\
 Data File : BP013102.D
 Acq On : 14 Dec 2022 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 13 03:29:24 2022

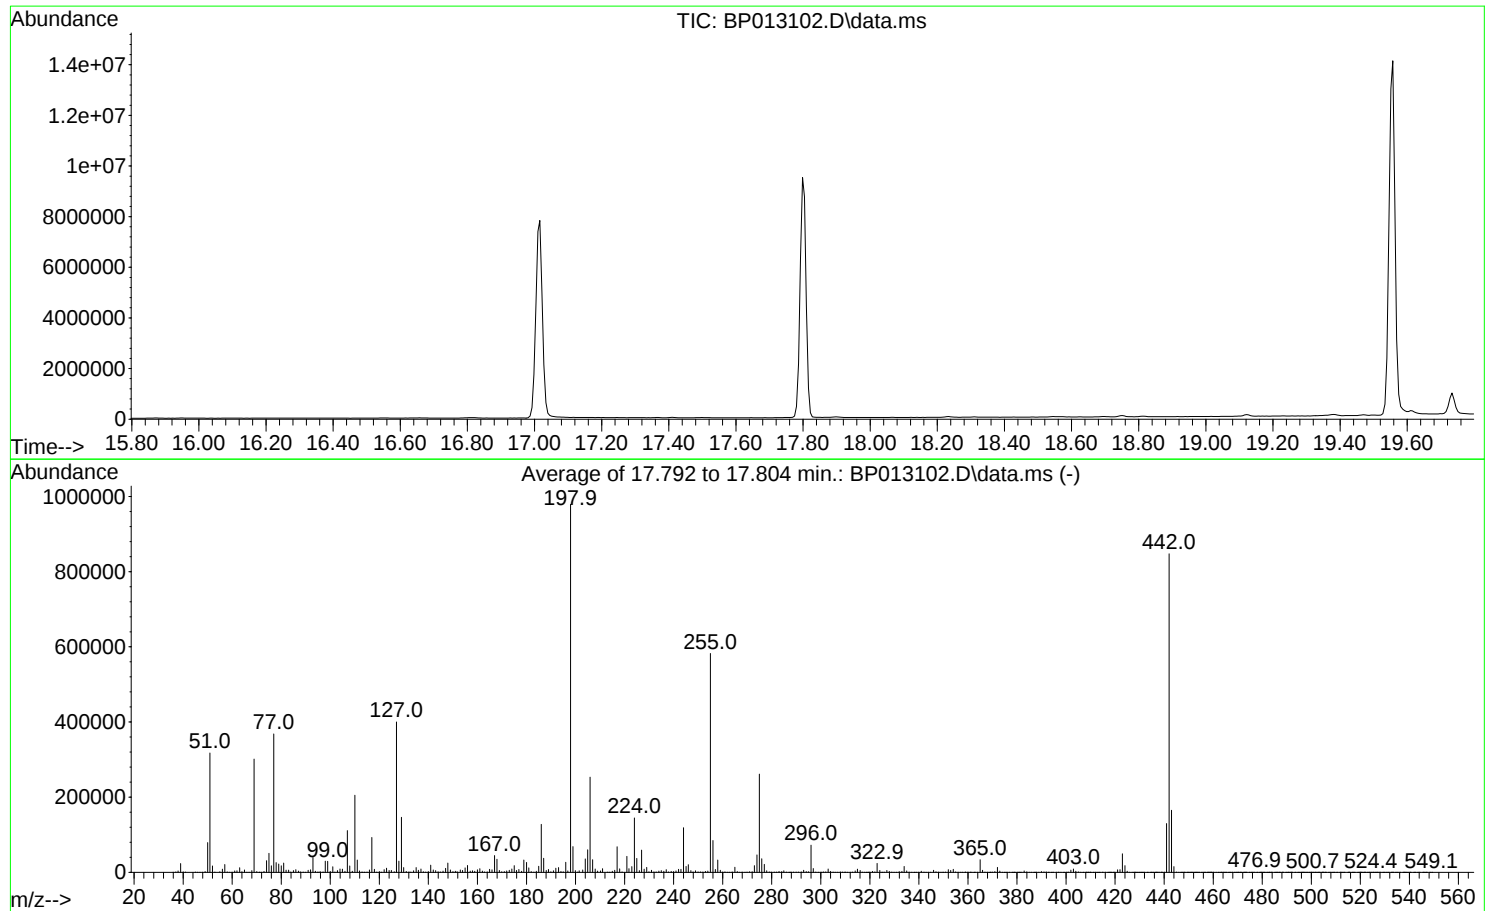




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	317463	PASS
68	69	0.00	2	1.5	4638	PASS
69	198	0.00	100	30.8	301125	PASS
70	69	0.00	2	0.6	1834	PASS
127	198	10	80	40.9	400214	PASS
197	198	0.00	2	0.4	3455	PASS
198	198	100	100	100.0	978983	PASS
199	198	5	9	7.0	68194	PASS
275	198	10	60	26.7	261468	PASS
365	198	1	100	3.4	33444	PASS
441	198	0.01	100	13.3	129877	PASS
442	442	100	100	100.0	847603	PASS
443	442	15	24	19.5	164896	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121422\
 Data File : BP013102.D
 Acq On : 14 Dec 2022 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 05:18:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

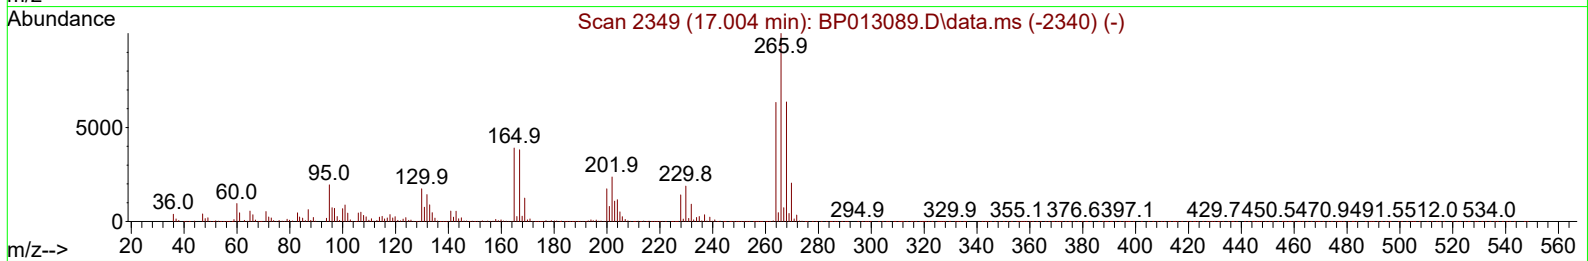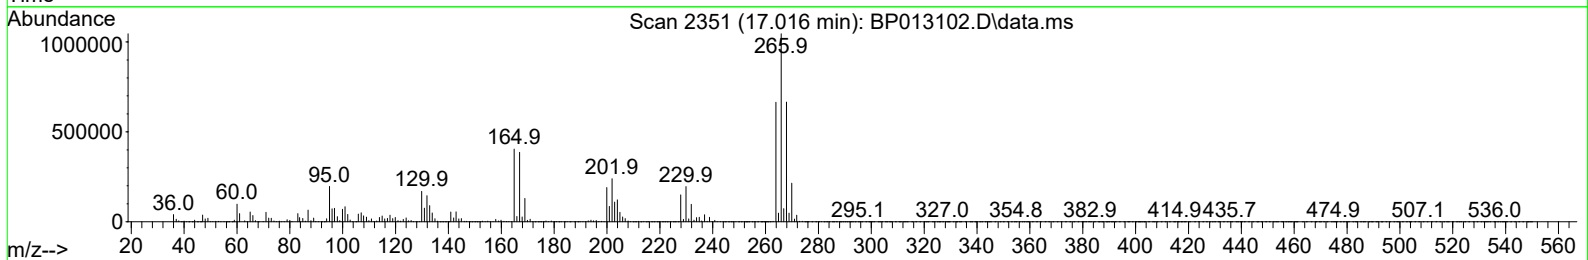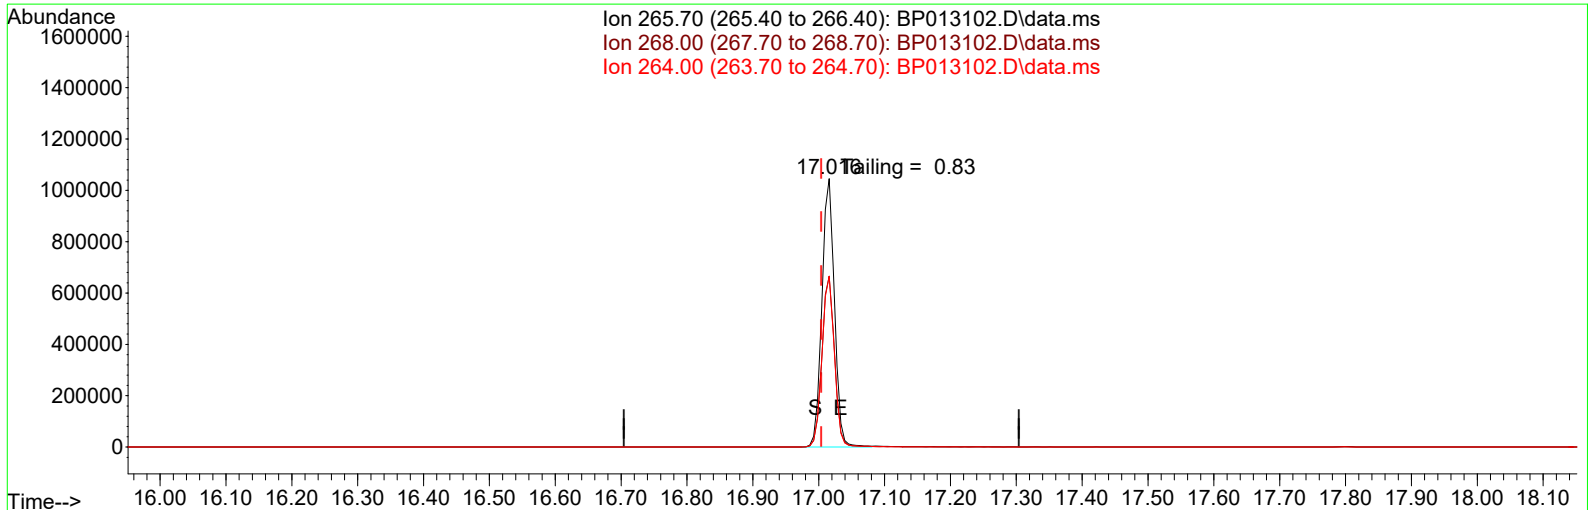

TIC: BP013102.D\data.ms

(70) Pentachlorophenol (C)

17.016min (+ 0.012) 35617.47 ng




response 1386707

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.66
264.00	63.30	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121422\
 Data File : BP013102.D
 Acq On : 14 Dec 2022 10:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 05:18:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

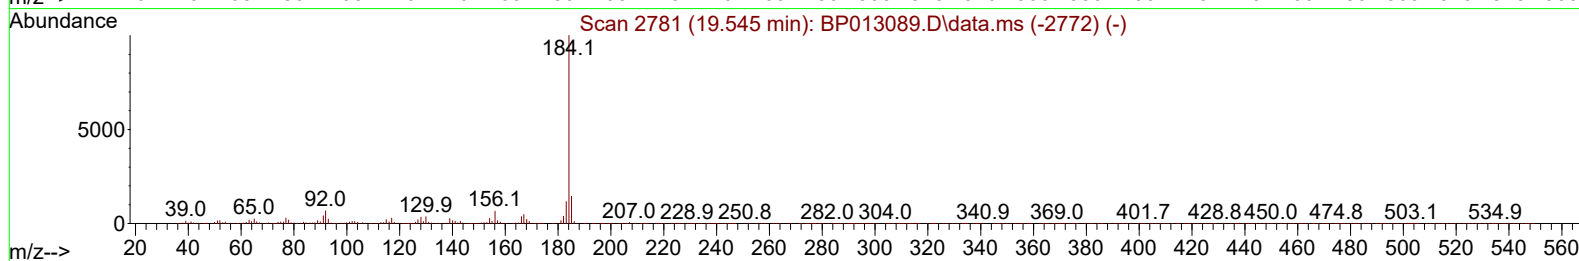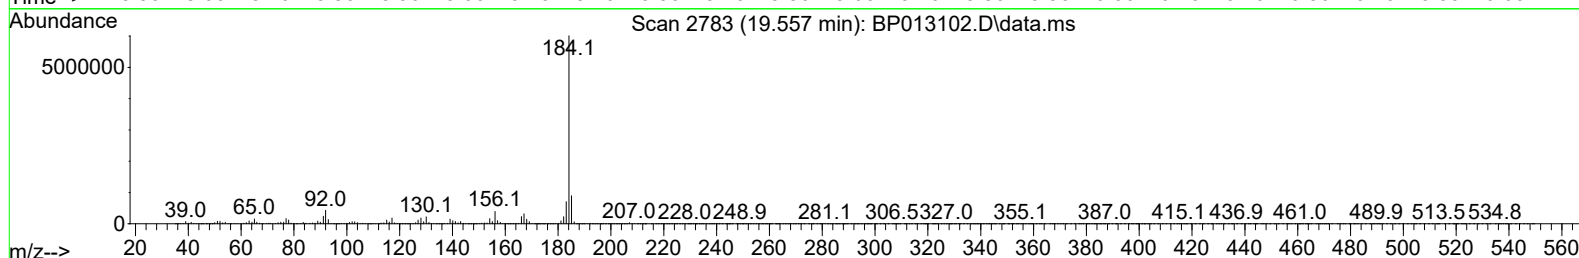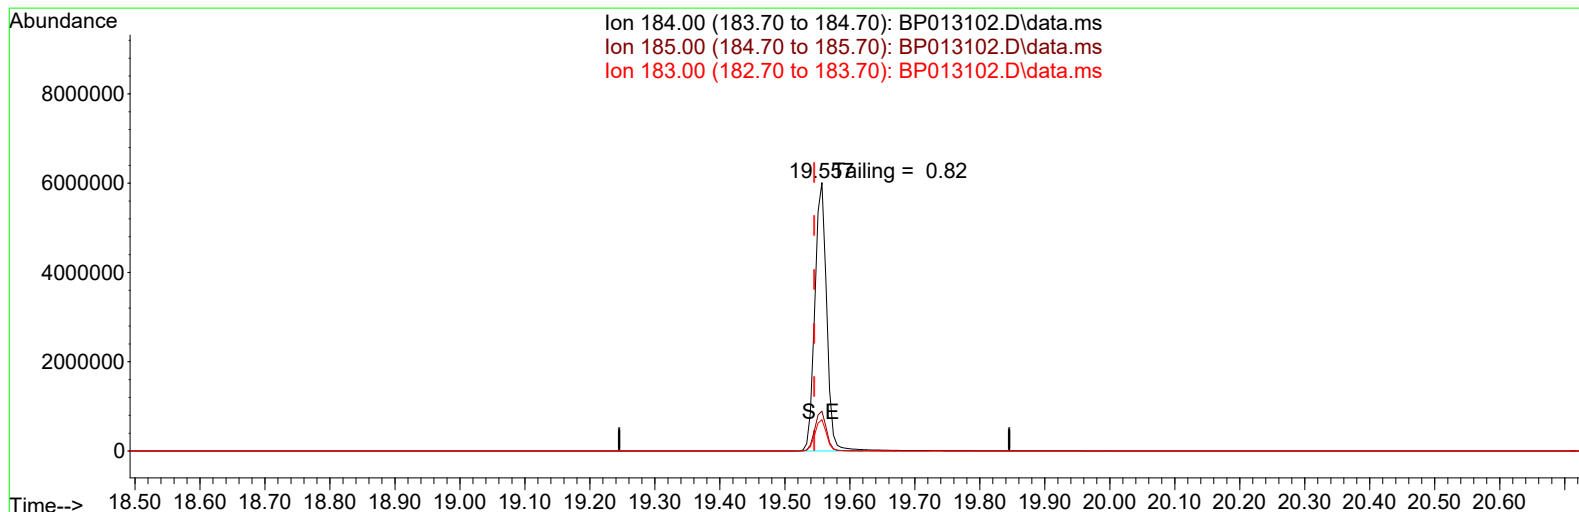

TIC: BP013102.D\data.ms

(77) Benzidine

19.557min (+ 0.012) 24878.84 ng

response 7670848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.87
183.00	11.70	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2022	BNA_P	<u>BP013102.D</u>
Compound Name	Response	Retention Time
DDT	3556903	20.751
DDD	34680	20.375
DDE	1216	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35896	3592799	1.00

Instrument :
BNA_P
ClientSampleId :
DFTPP