
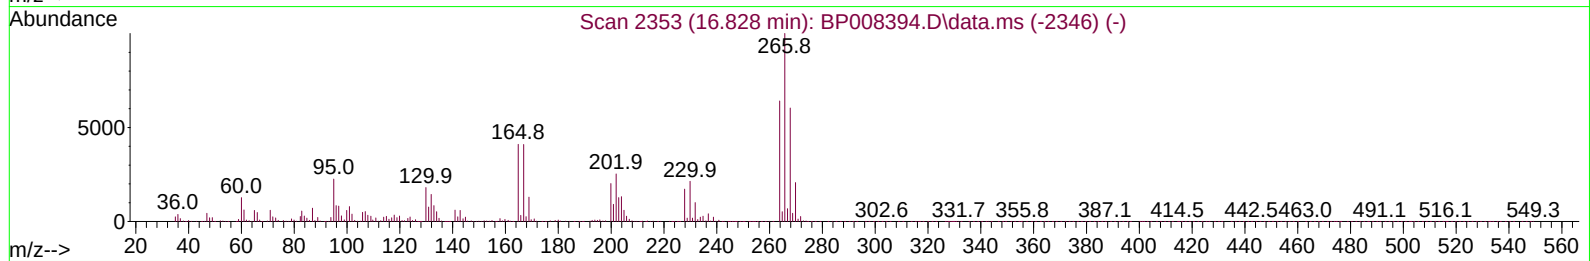
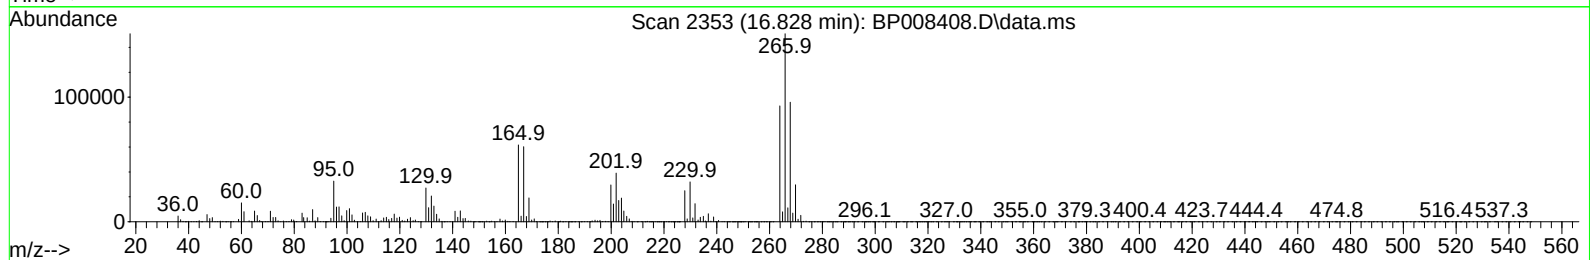


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008408.D
 Acq On : 15 Dec 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 16:15:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

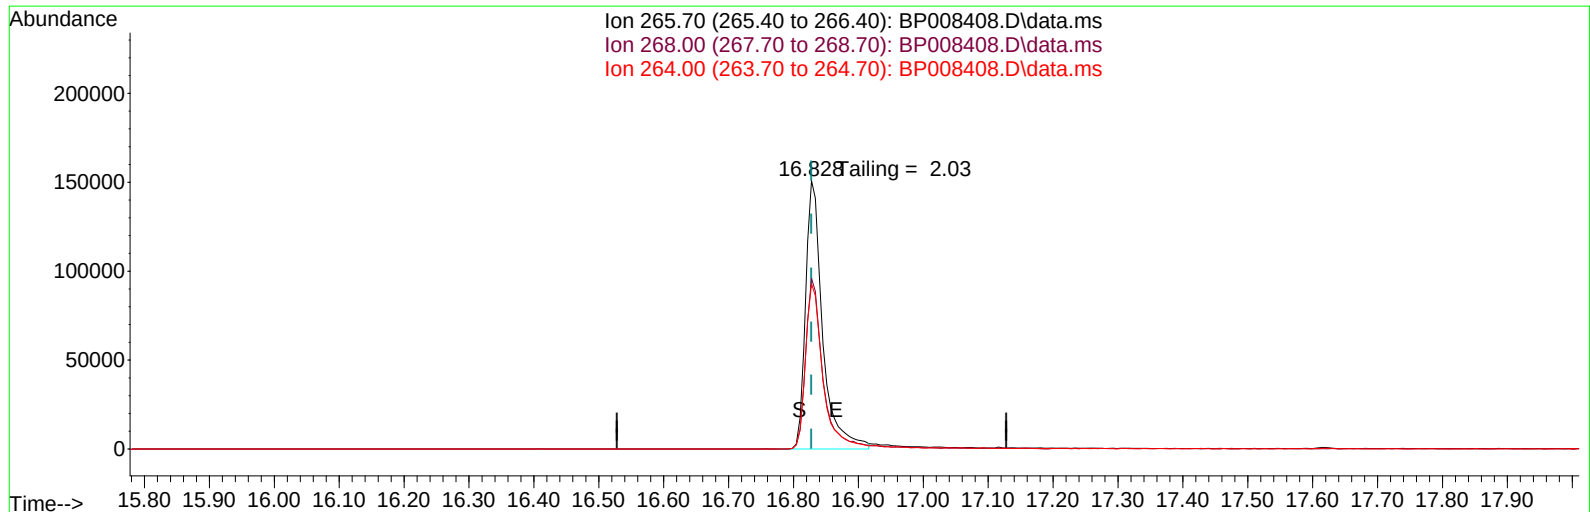

TIC: BP008408.D\data.ms

(70) Pentachlorophenol (C)




16.828min (+ 0.000) 969601.07 ng

response 285920

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.60
264.00	61.90	61.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008408.D
 Acq On : 15 Dec 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 16:15:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

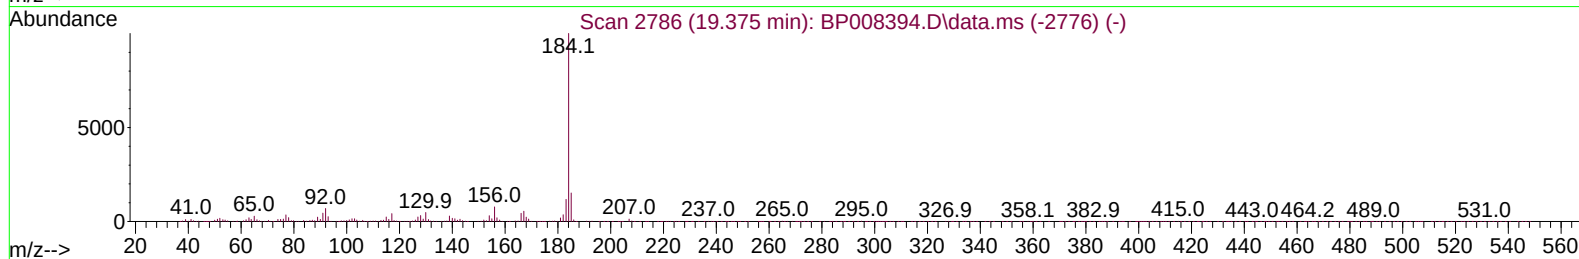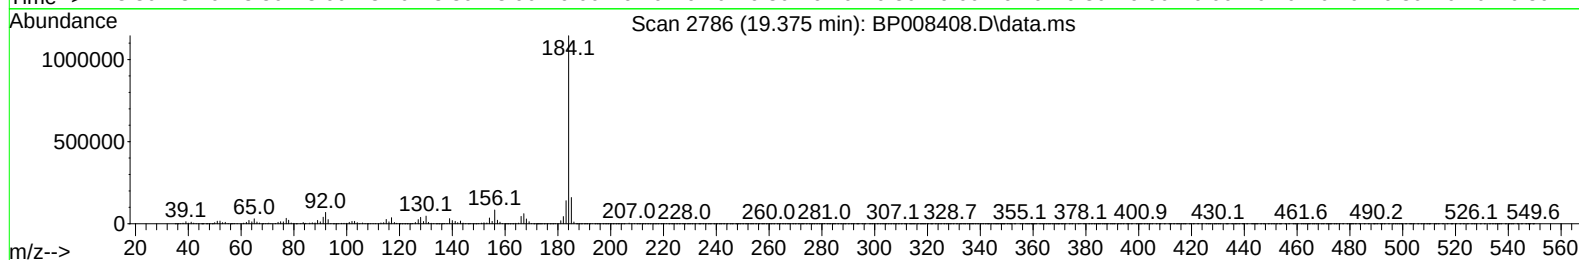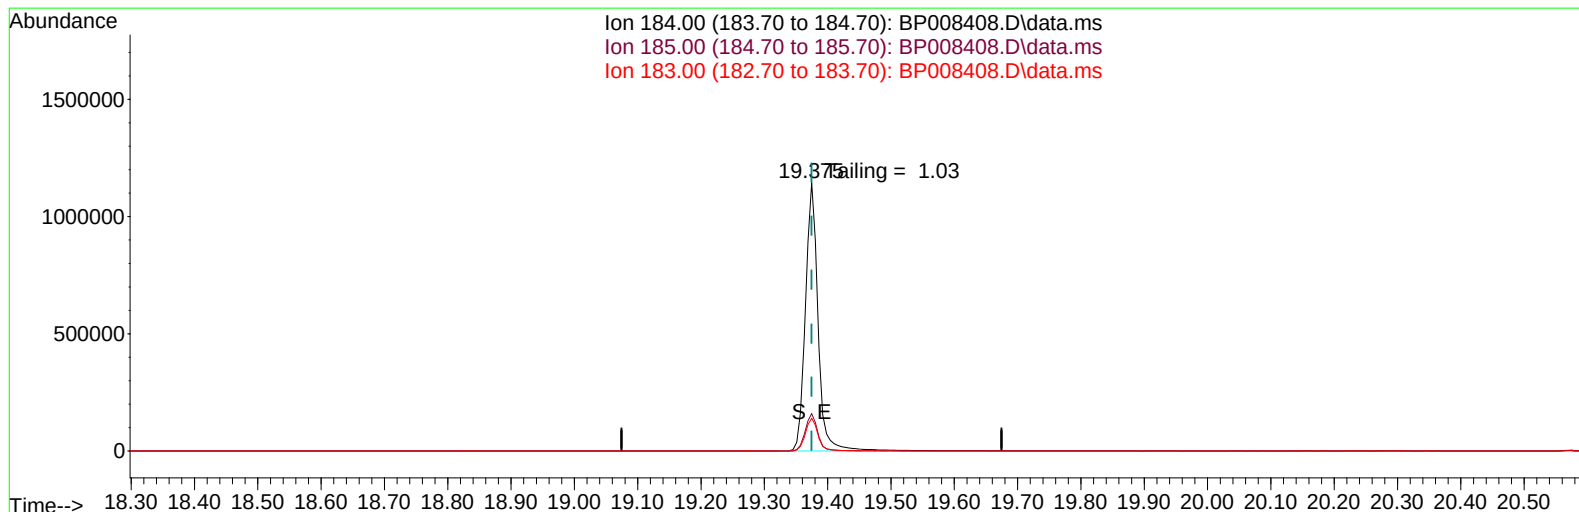

TIC: BP008408.D\data.ms

(77) Benzidine

19.375min (+ 0.000) 2046698.88 ng

response 1598570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.95
183.00	11.40	12.25
0.00	0.00	0.00