
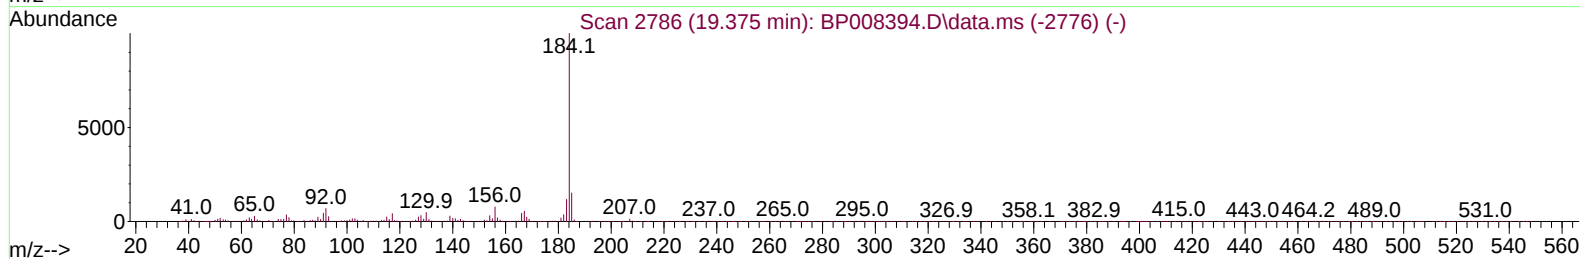
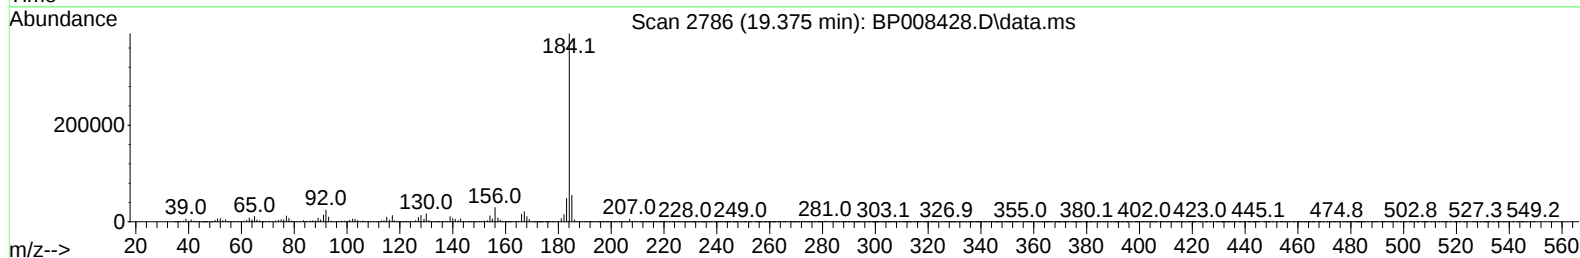


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008428.D
 Acq On : 15 Dec 2021 23:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 06:44:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

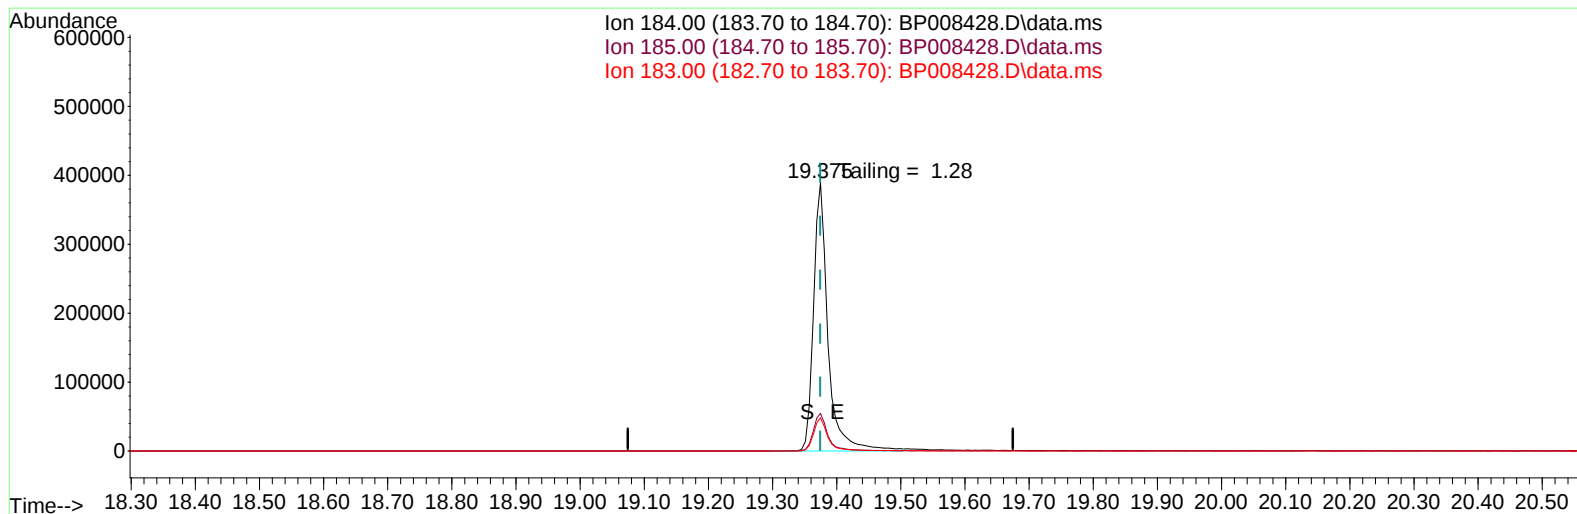




TIC: BP008428.D\data.ms

(77) Benzidine**19.375min (+ 0.000) 30208.92 ng****response 617750**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.01
183.00	11.40	12.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008428.D
Acq On : 15 Dec 2021 23:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 06:44:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 17:59:47 2021
Response via : Initial Calibration

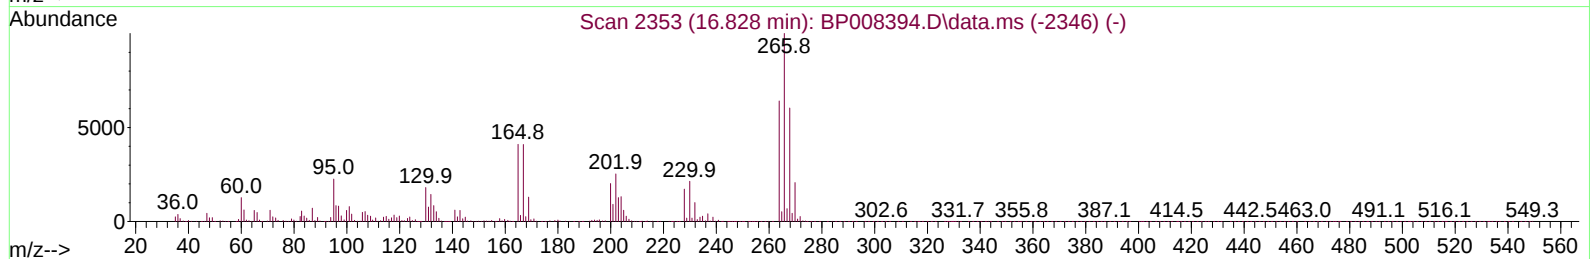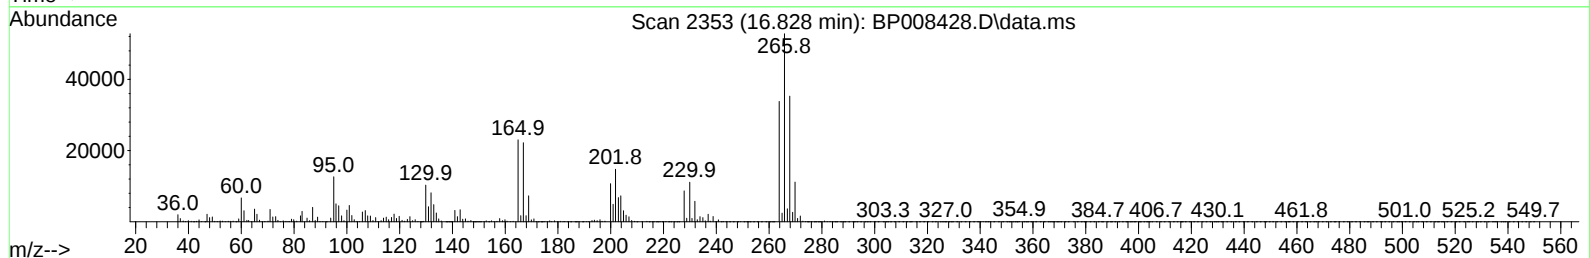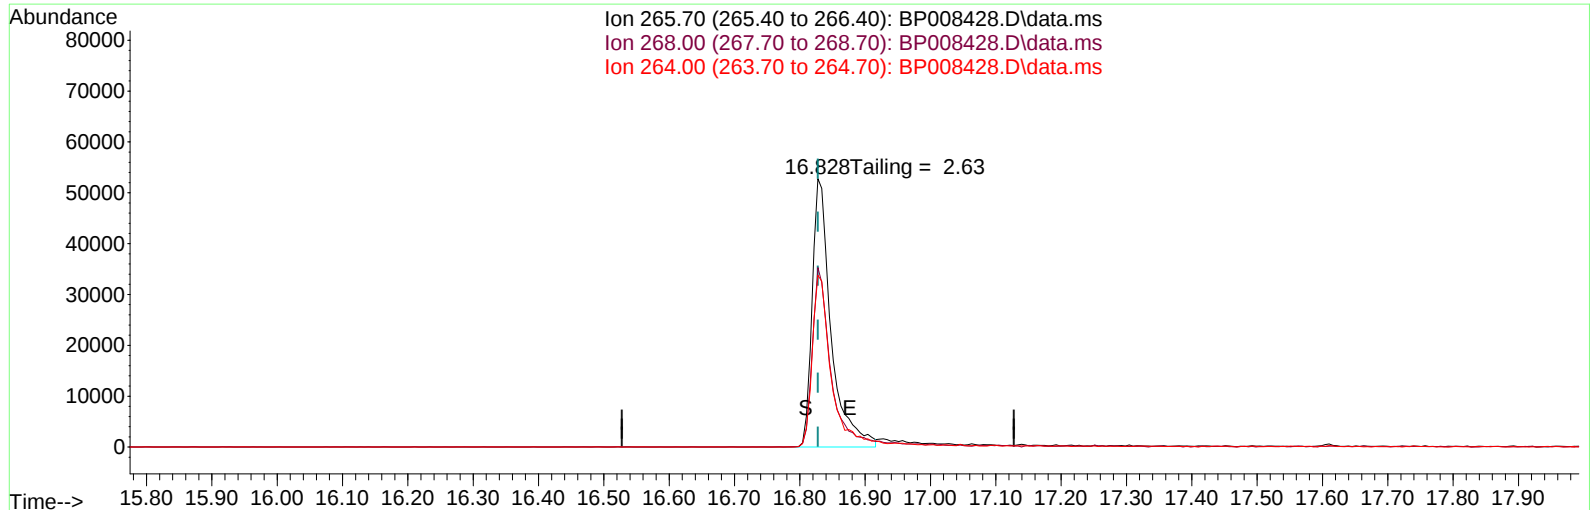

TIC: BP008428.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.000) 222676.66 ng

response 111343

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.84
264.00	61.90	63.97
0.00	0.00	0.00