

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008427.D
 Acq On : 15 Dec 2021 20:57
 Operator : CG/JU
 Sample : M5065-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 UV-1WC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.940	159	162	173	rVB2	12431	21250	1.29%	0.176%
2	4.875	317	321	329	rBV	39797	58232	3.54%	0.482%
3	5.346	396	401	417	rBV	124438	222679	13.54%	1.844%
4	6.952	668	674	690	rBV	95582	218775	13.31%	1.812%
5	7.740	801	808	819	rBV	254312	416306	25.32%	3.447%
6	8.581	945	951	961	rBV6	6803	25160	1.53%	0.208%
7	8.910	1001	1007	1015	rBV	66627	138238	8.41%	1.145%
8	10.540	1272	1284	1290	rBV	305865	544262	33.10%	4.507%
9	10.587	1290	1292	1301	rVB2	21571	32199	1.96%	0.267%
10	12.216	1563	1569	1574	rVB	9773	17056	1.04%	0.141%
11	13.016	1695	1705	1715	rBV	189741	309809	18.84%	2.565%
12	13.575	1790	1800	1806	rBV	5801	16631	1.01%	0.138%
13	14.122	1889	1893	1902	rVB2	14667	25636	1.56%	0.212%
14	14.393	1932	1939	1946	rBV	455394	723612	44.01%	5.992%
15	14.457	1946	1950	1960	rVB	41087	71835	4.37%	0.595%
16	14.804	2004	2009	2014	rVB	20431	29761	1.81%	0.246%
17	15.451	2114	2119	2131	rVB	48326	81324	4.95%	0.673%
18	15.751	2166	2170	2177	rVB2	16313	26699	1.62%	0.221%
19	15.904	2190	2196	2203	rBV	164373	266734	16.22%	2.209%
20	16.145	2234	2237	2242	rVB4	20910	28649	1.74%	0.237%
21	16.463	2286	2291	2295	rBV3	12110	23857	1.45%	0.198%
22	16.975	2374	2378	2387	rVB2	36677	64052	3.90%	0.530%
23	17.157	2403	2409	2413	rBV	602292	872545	53.07%	7.225%
24	17.198	2413	2416	2422	rVB	283368	398752	24.25%	3.302%
25	17.292	2428	2432	2438	rVB	83781	119590	7.27%	0.990%
26	17.581	2476	2481	2486	rBV2	34328	65503	3.98%	0.542%
27	17.775	2511	2514	2518	rVB	52270	68353	4.16%	0.566%
28	18.033	2554	2558	2561	rBV	43866	65474	3.98%	0.542%
29	18.081	2561	2566	2571	rVB2	69986	130728	7.95%	1.083%
30	18.157	2577	2579	2583	rVB2	27767	33987	2.07%	0.281%
31	18.222	2586	2590	2594	rBV2	66108	103829	6.32%	0.860%
32	18.516	2637	2640	2645	rBV	39966	54196	3.30%	0.449%
33	19.180	2749	2753	2758	rBV	535019	666521	40.54%	5.519%
34	19.510	2805	2809	2810	rBV2	104949	135695	8.25%	1.124%
35	19.533	2810	2813	2822	rVB	390464	558355	33.96%	4.624%
36	19.728	2842	2846	2851	rVB	384249	478334	29.09%	3.961%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008427.D
Acq On : 15 Dec 2021 20:57
Operator : CG/JU
Sample : M5065-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
UV-1WC

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.269	3102	3108	3111	rBV2	835497	1332824	81.07%	11.037%
38	21.380	3123	3127	3139	rVB	722033	1031289	62.73%	8.540%
39	23.633	3506	3510	3517	rVB2	512747	953536	58.00%	7.896%
40	26.104	3924	3930	3943	rVB4	568573	1644098	100.00%	13.614%




Sum of corrected areas: 12076365

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008427.D
Acq On : 15 Dec 2021 20:57
Operator : CG/JU
Sample : M5065-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

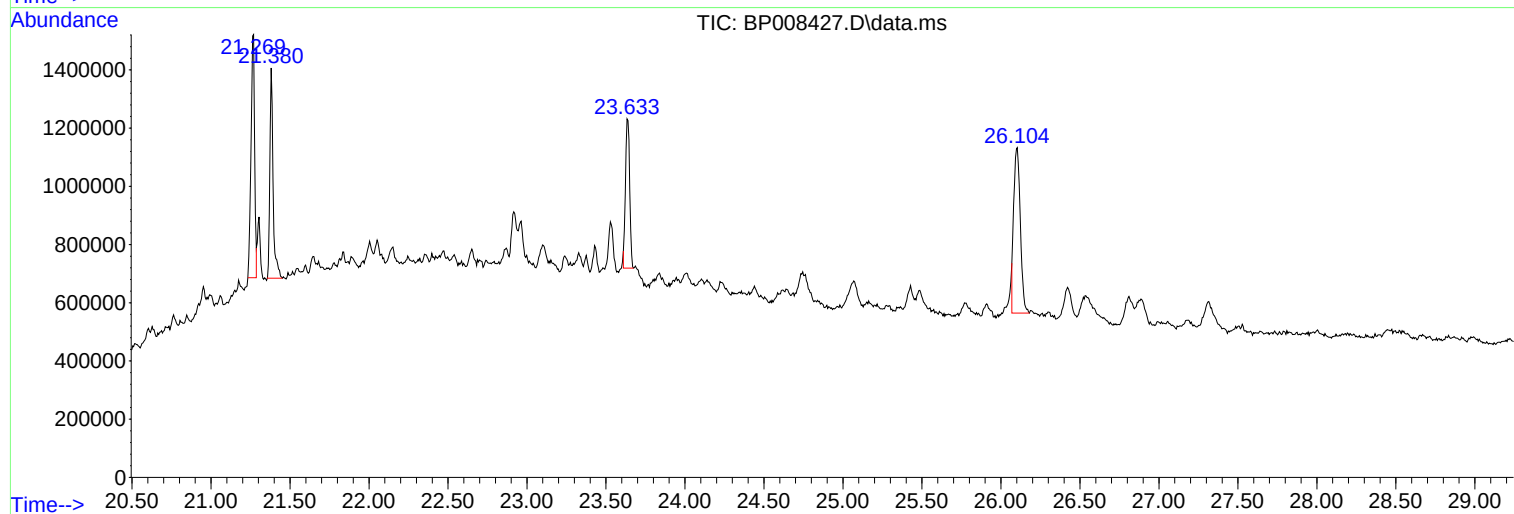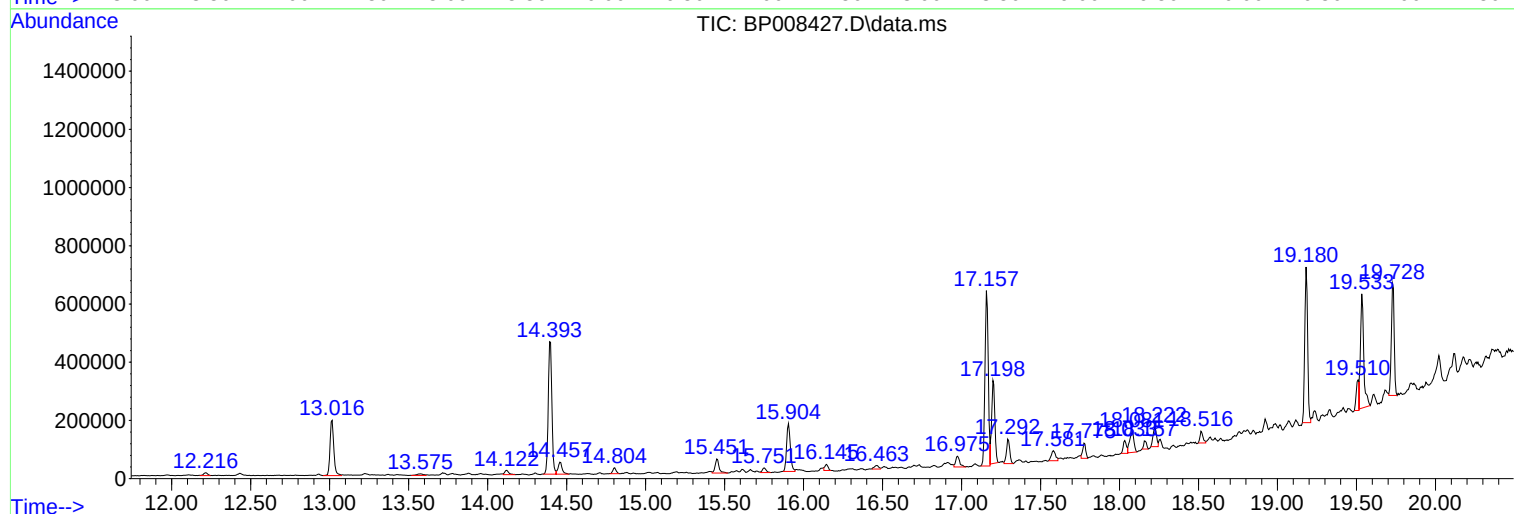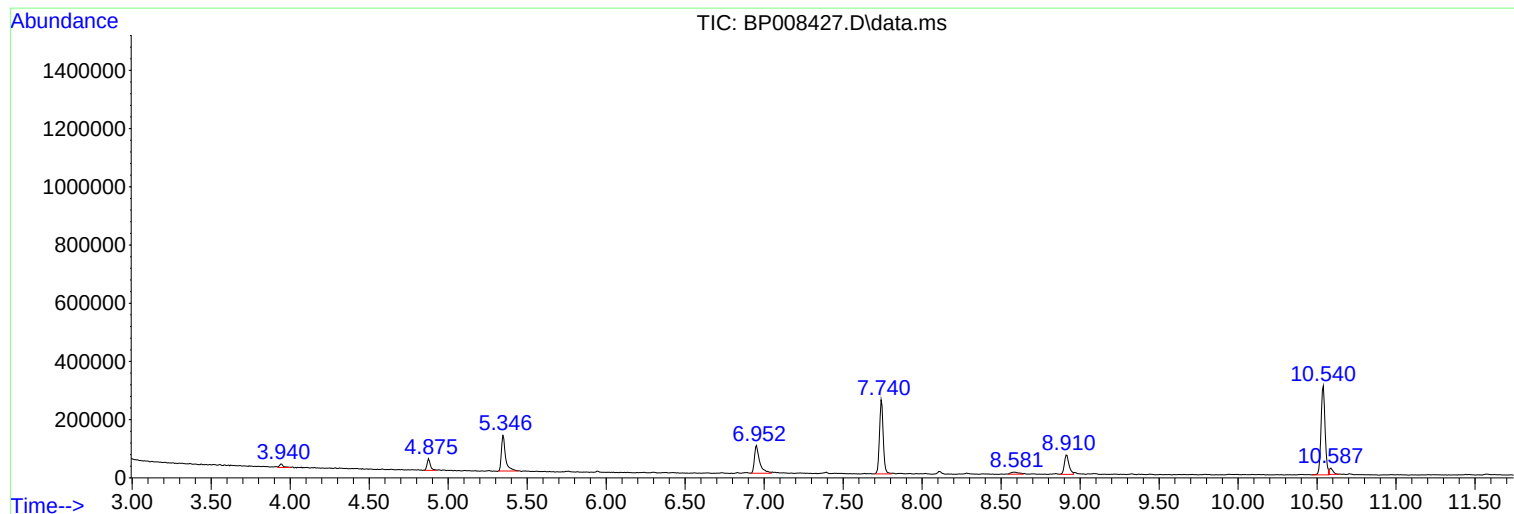

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008427.D
Acq On : 15 Dec 2021 20:57
Operator : CG/JU
Sample : M5065-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008427.D
Acq On : 15 Dec 2021 20:57
Operator : CG/JU
Sample : M5065-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------