

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008430.D
 Acq On : 16 Dec 2021 00:35
 Operator : CG/JU
 Sample : PB141409BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141409BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.346	395	401	419	rBV	950888	1496839	39.84%	9.342%
2	6.940	666	672	689	rBV	803459	1488098	39.61%	9.288%
3	7.740	802	808	819	rBV	165028	269729	7.18%	1.683%
4	8.910	999	1007	1031	rBV	536103	994813	26.48%	6.209%
5	10.540	1277	1284	1299	rBV	194621	359607	9.57%	2.244%
6	13.016	1697	1705	1722	rBV	1364816	2115739	56.32%	13.205%
7	14.398	1931	1940	1956	rBV	291773	496943	13.23%	3.102%
8	15.904	2189	2196	2221	rBV	984619	1790457	47.66%	11.175%
9	17.163	2404	2410	2425	rBV	376874	614690	16.36%	3.836%
10	19.733	2842	2847	2860	rBV	3008464	3756956	100.00%	23.448%
11	21.269	3103	3108	3113	rBV	608073	826765	22.01%	5.160%
12	21.386	3123	3128	3139	rBV	654940	980524	26.10%	6.120%
13	23.639	3506	3511	3522	rVB2	391004	831060	22.12%	5.187%




Sum of corrected areas: 16022220

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008430.D
Acq On : 16 Dec 2021 00:35
Operator : CG/JU
Sample : PB141409BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141409BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

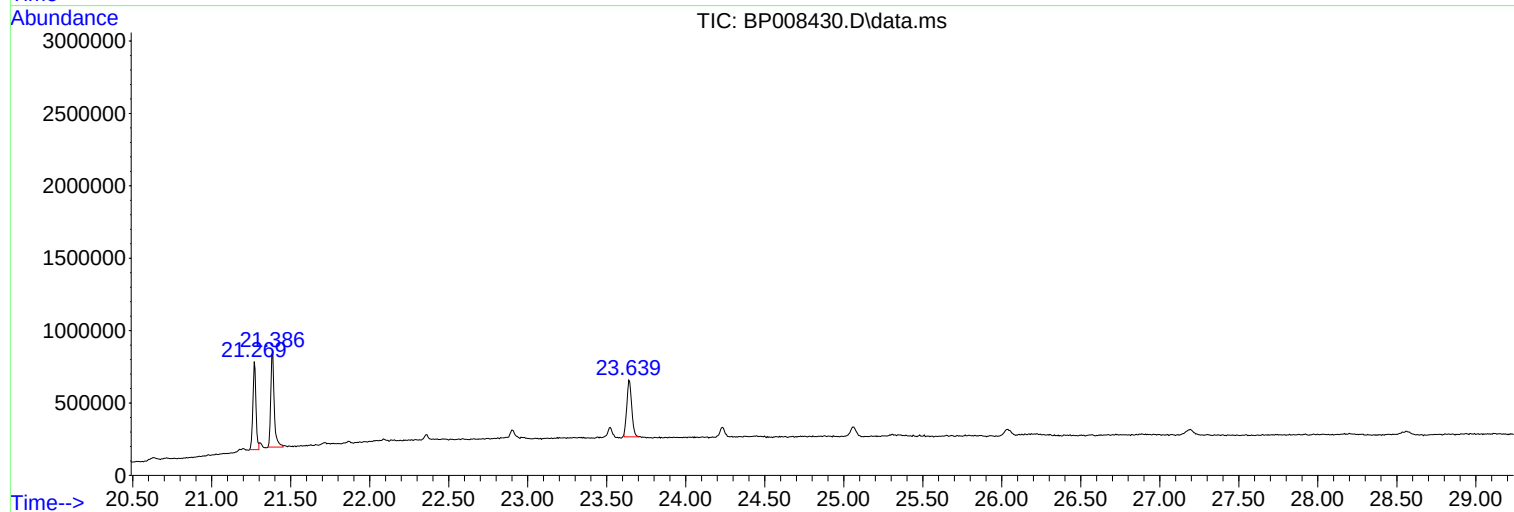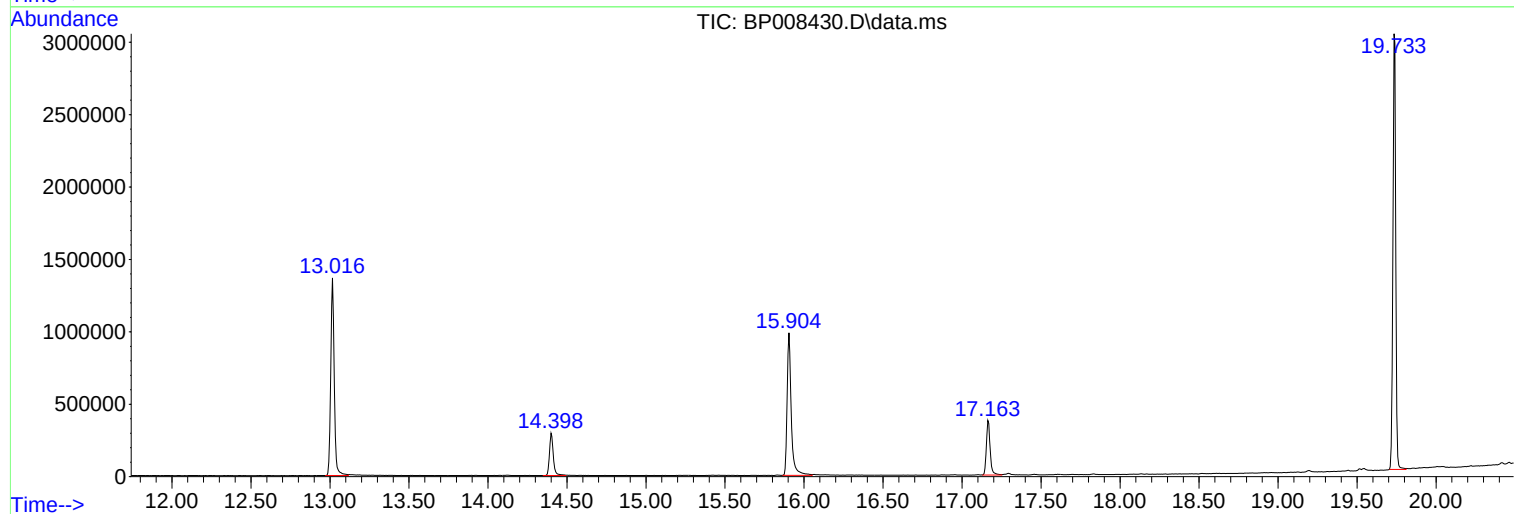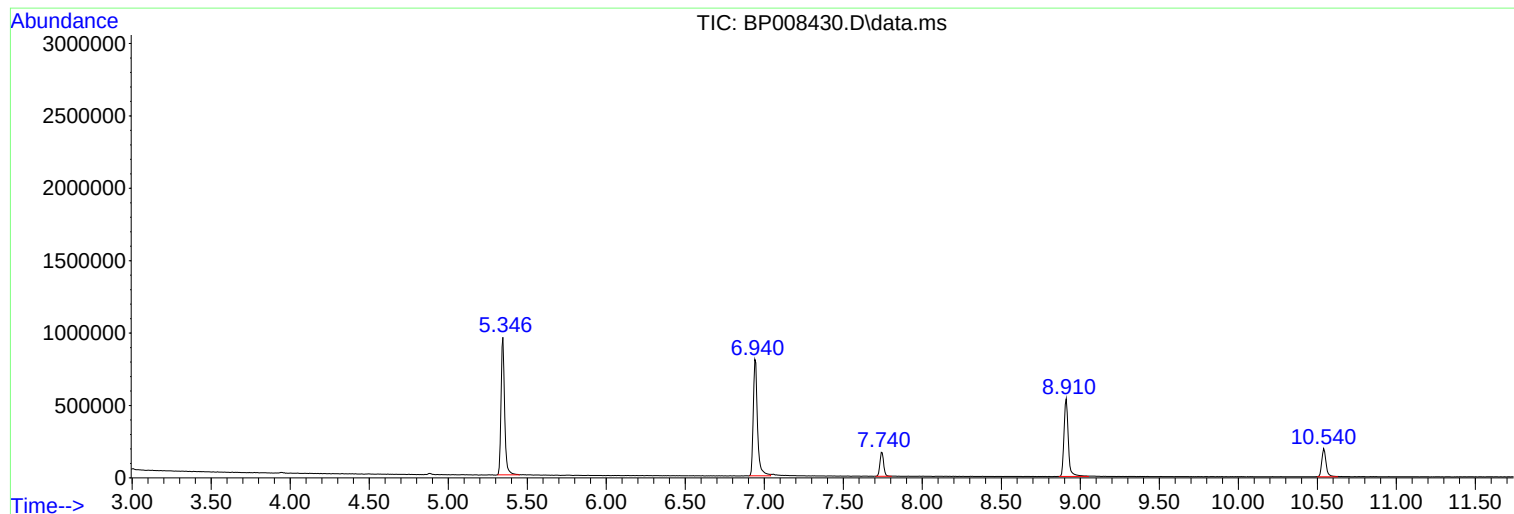

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008430.D
Acq On : 16 Dec 2021 00:35
Operator : CG/JU
Sample : PB141409BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141409BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.386	23.72 ng	980524	Chrysene-d12	21.269

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	49
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	32
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	25

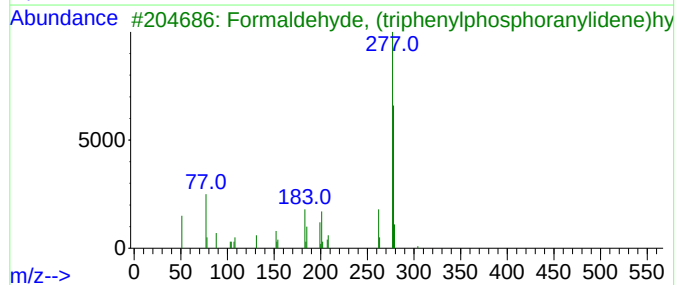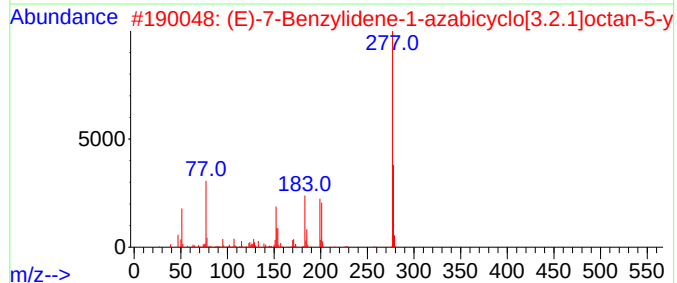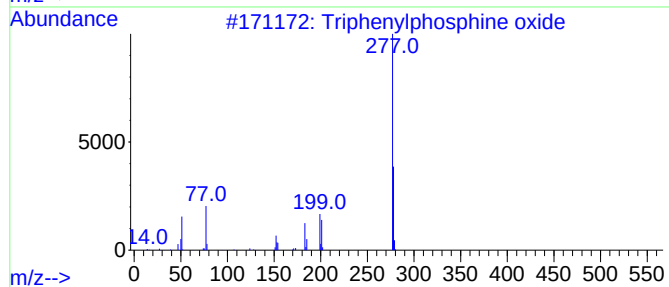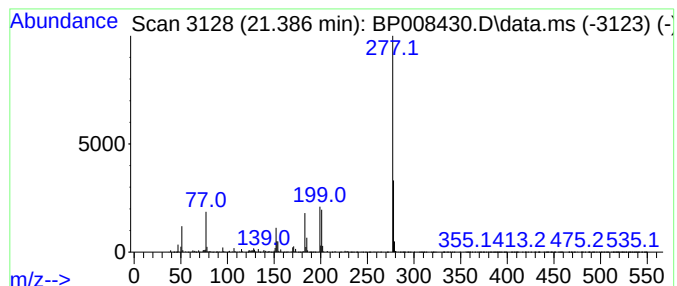

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
Data File : BP008430.D
Acq On : 16 Dec 2021 00:35
Operator : CG/JU
Sample : PB141409BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141409BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.386	23.7	ng	980524	5	21.269	826765	20.0