
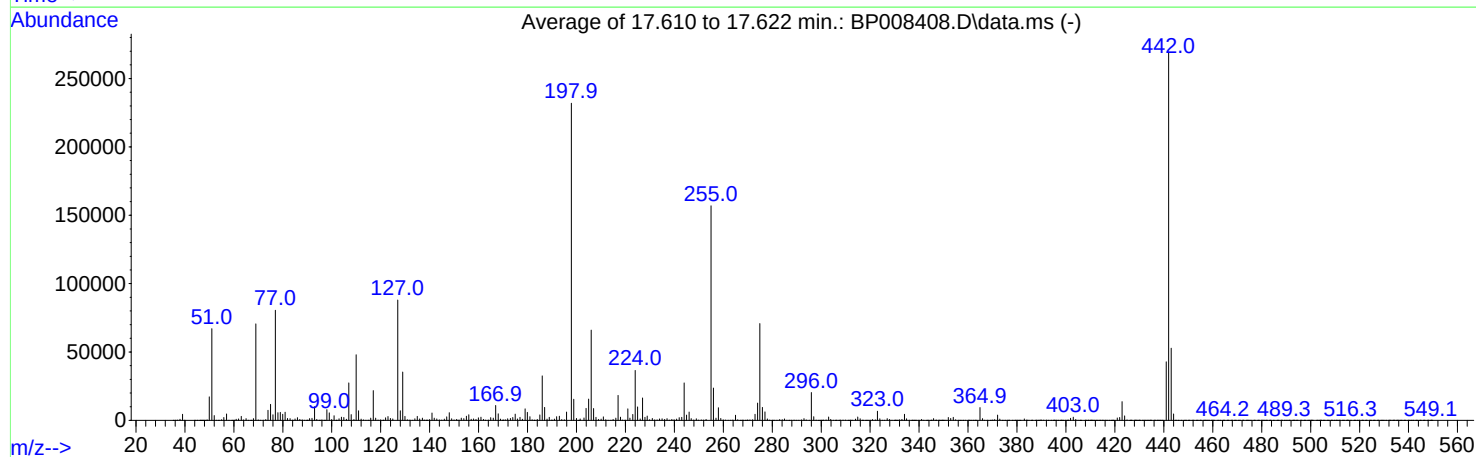


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008408.D
 Acq On : 15 Dec 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 17:59:47 2021

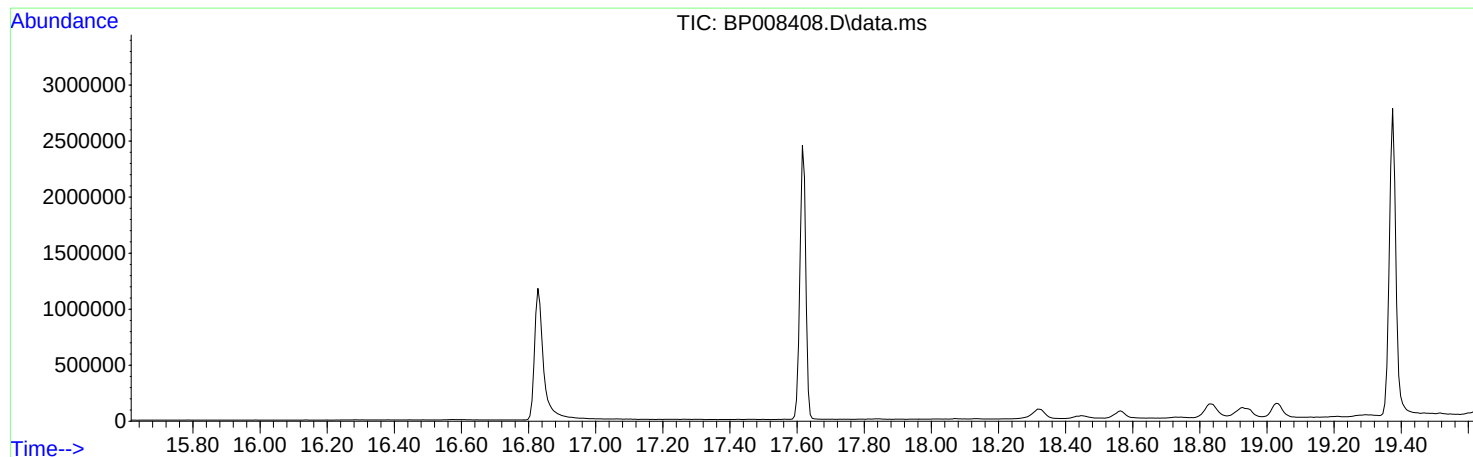

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	67025	PASS
68	69	0.00	2	1.9	1330	PASS
69	198	0.00	100	30.4	70616	PASS
70	69	0.00	2	0.5	370	PASS
127	198	10	80	38.0	88045	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	231911	PASS
199	198	5	9	6.7	15504	PASS
275	198	10	60	30.5	70762	PASS
365	198	1	100	4.0	9352	PASS
441	198	0.01	100	18.5	42813	PASS
442	442	100	100	100.0	269035	PASS
443	442	15	24	19.6	52742	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
12/15/2021	BNA_P	<u>BP008408.D</u>
Compound Name	Response	Retention Time
DDT	843129	20.575
DDD	14775	20.145
DDE	1760	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16535	859664	1.92

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008408.D
 Acq On : 15 Dec 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 16:15:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

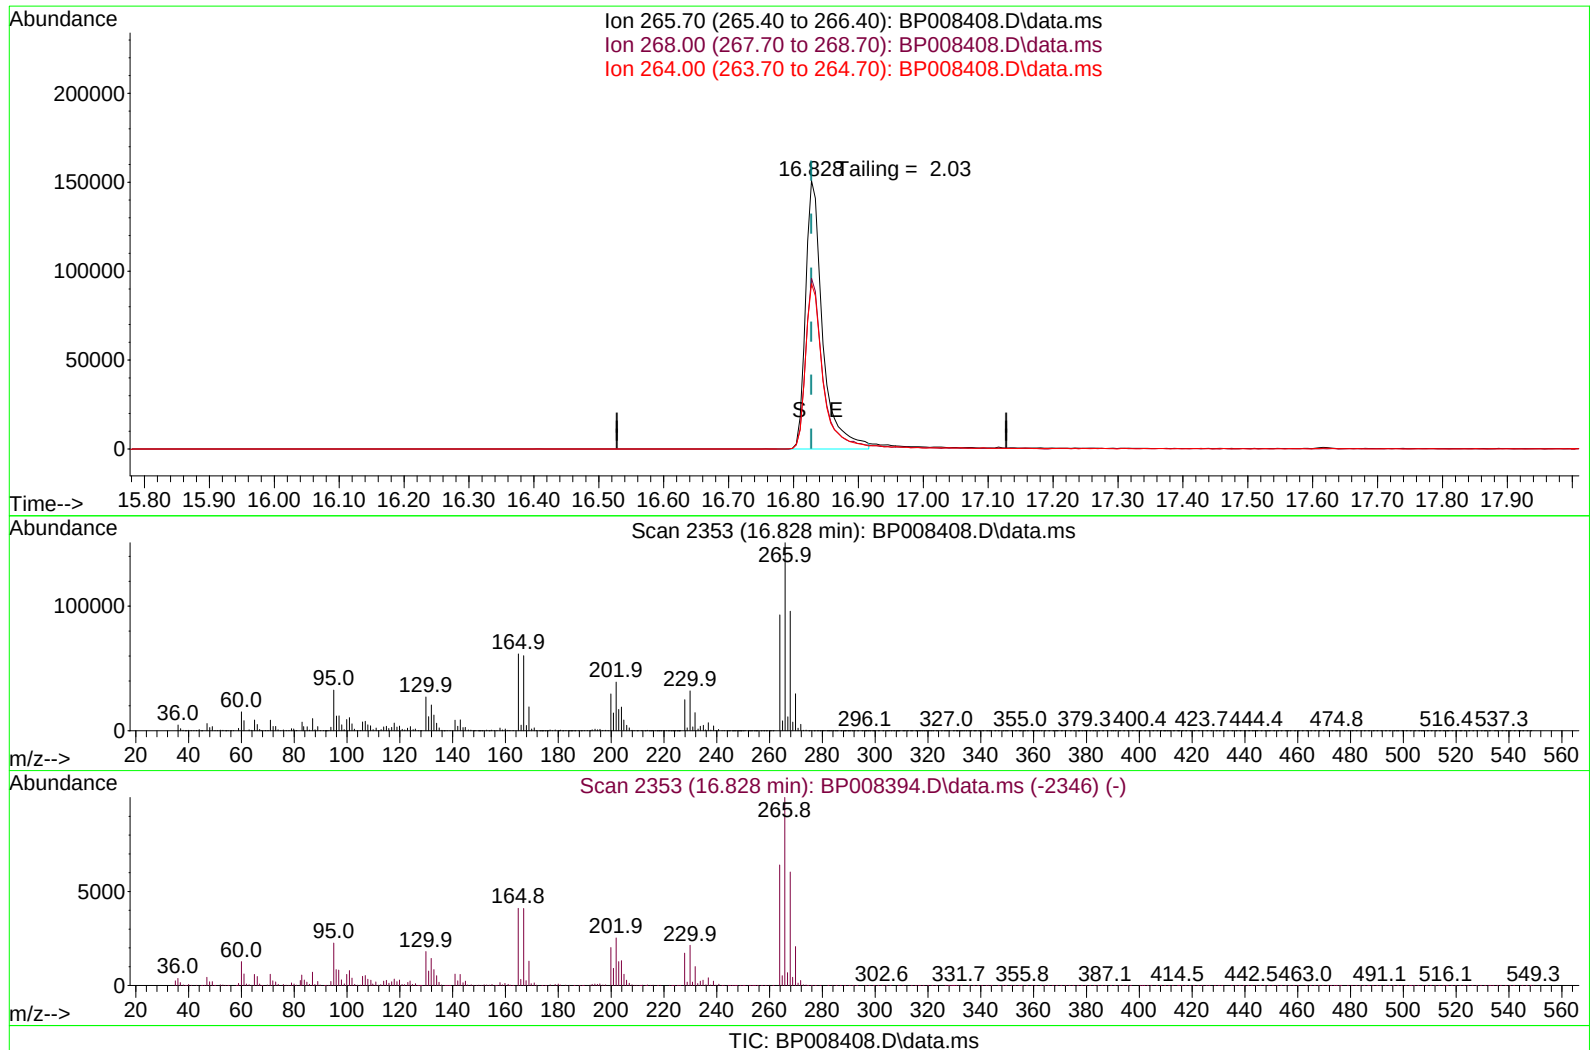

TIC: BP008408.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.000) 969601.07 ng




response 285920

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.60
264.00	61.90	61.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008408.D
 Acq On : 15 Dec 2021 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 16:15:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

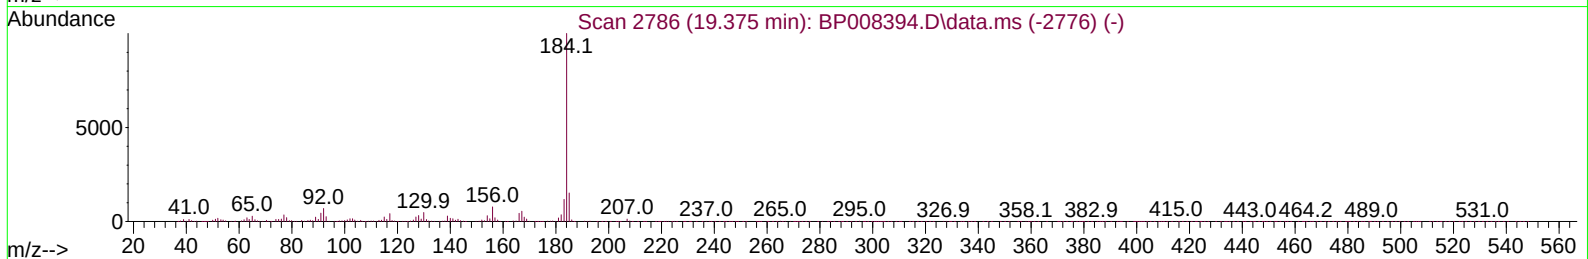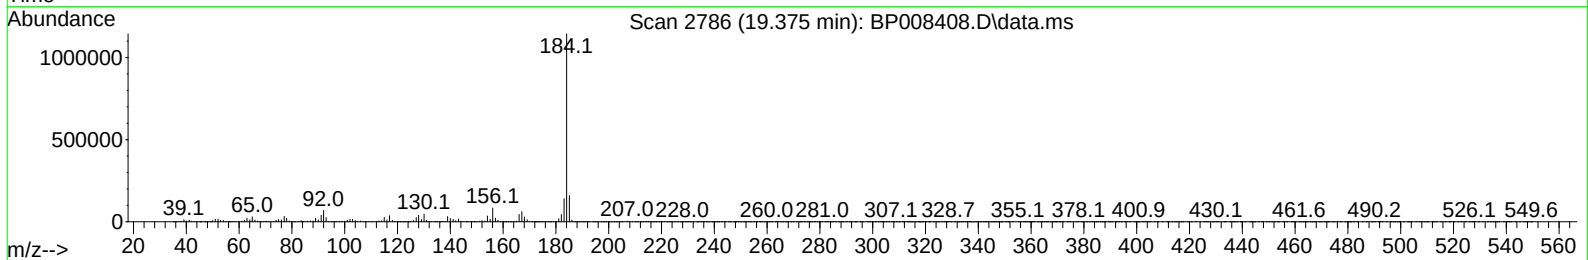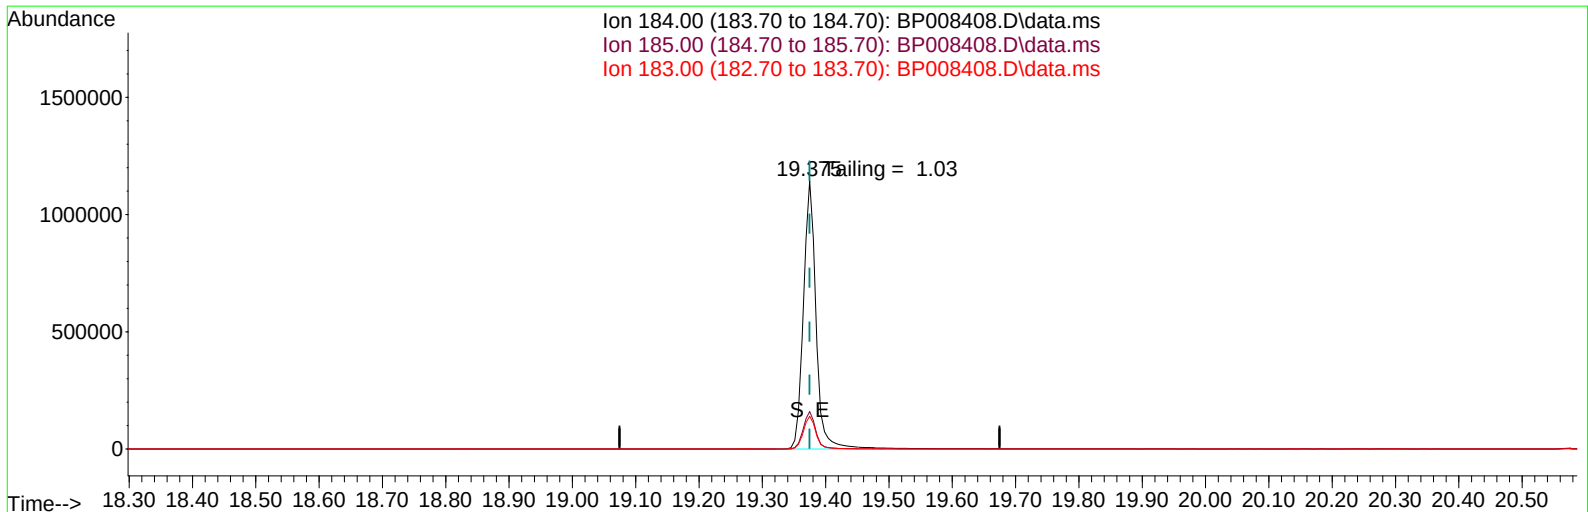

TIC: BP008408.D\data.ms

(77) Benzidine

19.375min (+ 0.000) 2046698.88 ng

response 1598570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.95
183.00	11.40	12.25
0.00	0.00	0.00