
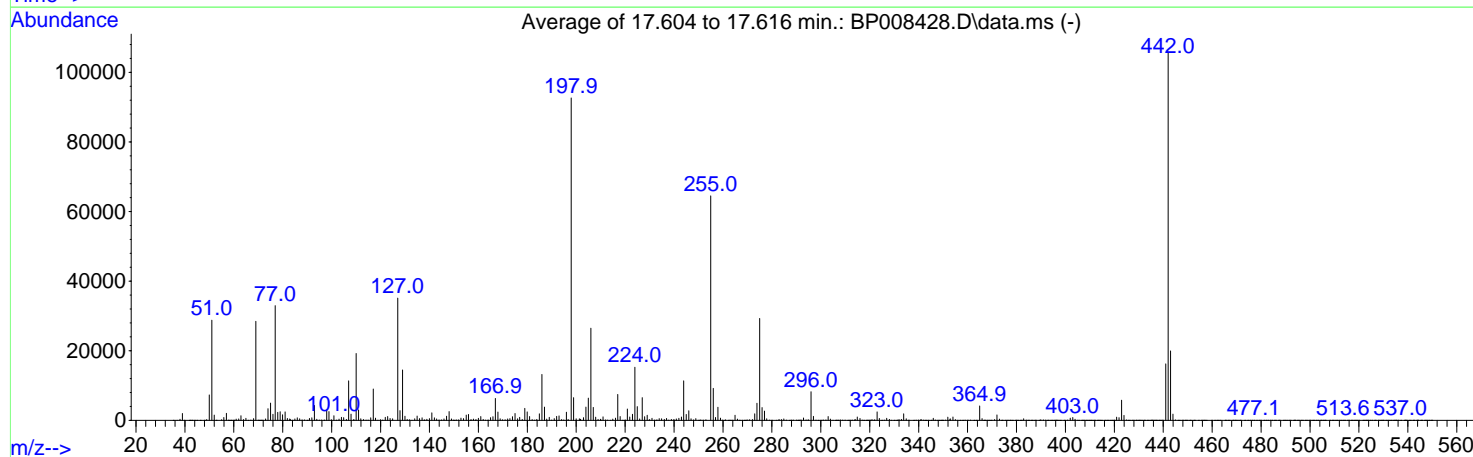


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008428.D
 Acq On : 15 Dec 2021 23:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 17:59:47 2021

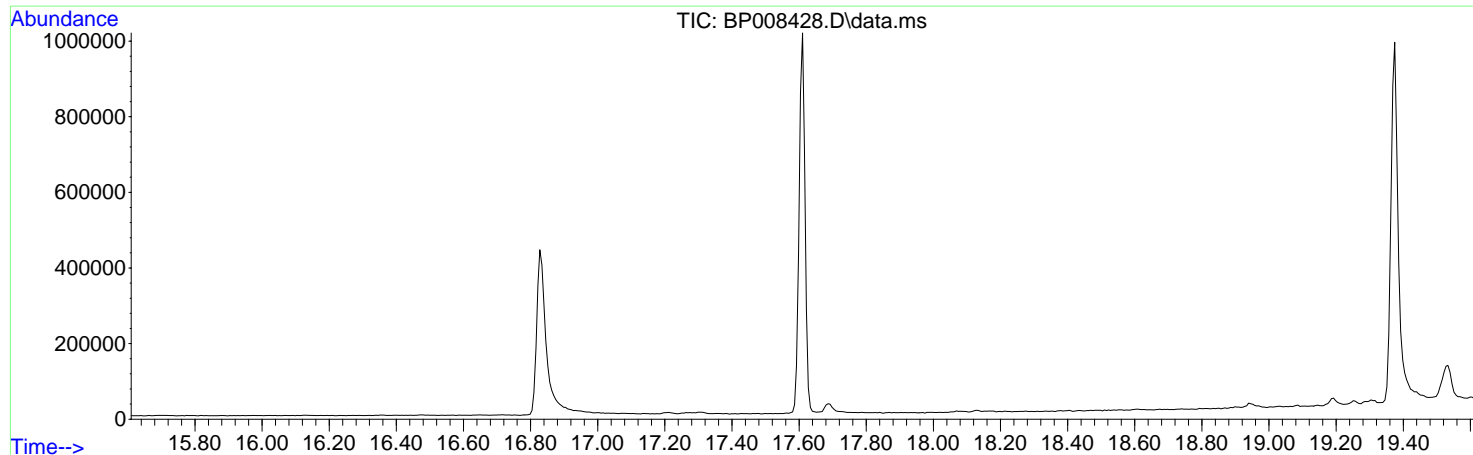




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	28788	PASS
68	69	0.00	2	1.9	528	PASS
69	198	0.00	100	30.7	28454	PASS
70	69	0.00	2	0.4	104	PASS
127	198	10	80	37.9	35133	PASS
197	198	0.00	2	0.3	298	PASS
198	198	100	100	100.0	92639	PASS
199	198	5	9	7.1	6536	PASS
275	198	10	60	31.6	29272	PASS
365	198	1	100	4.4	4116	PASS
441	198	0.01	100	17.5	16239	PASS
442	442	100	100	100.0	105688	PASS
443	442	15	24	18.9	19949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008428.D
 Acq On : 15 Dec 2021 23:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DFTPP

Quant Time: Dec 16 06:44:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

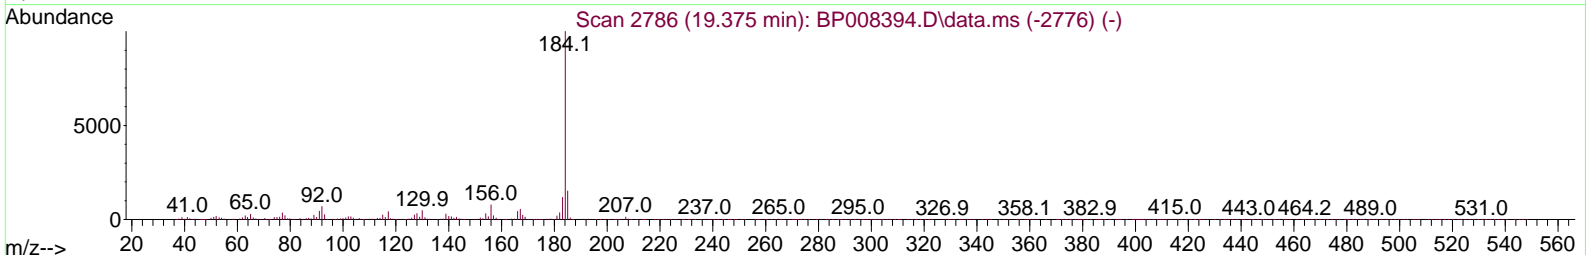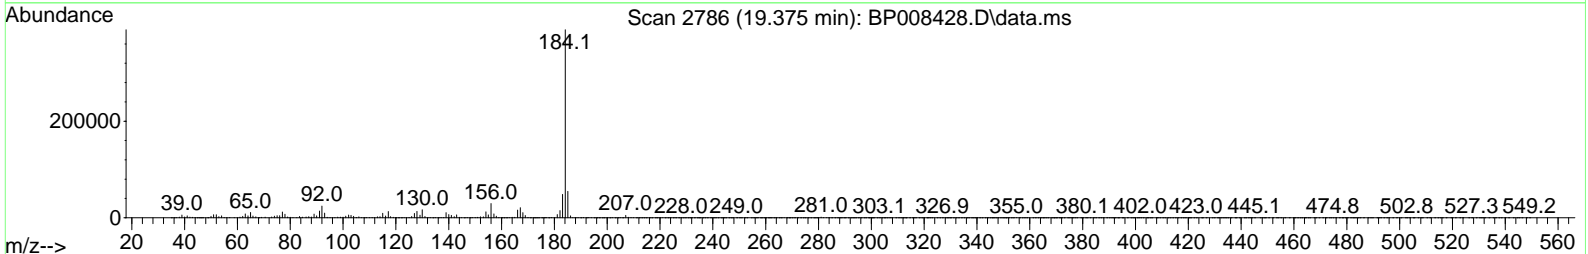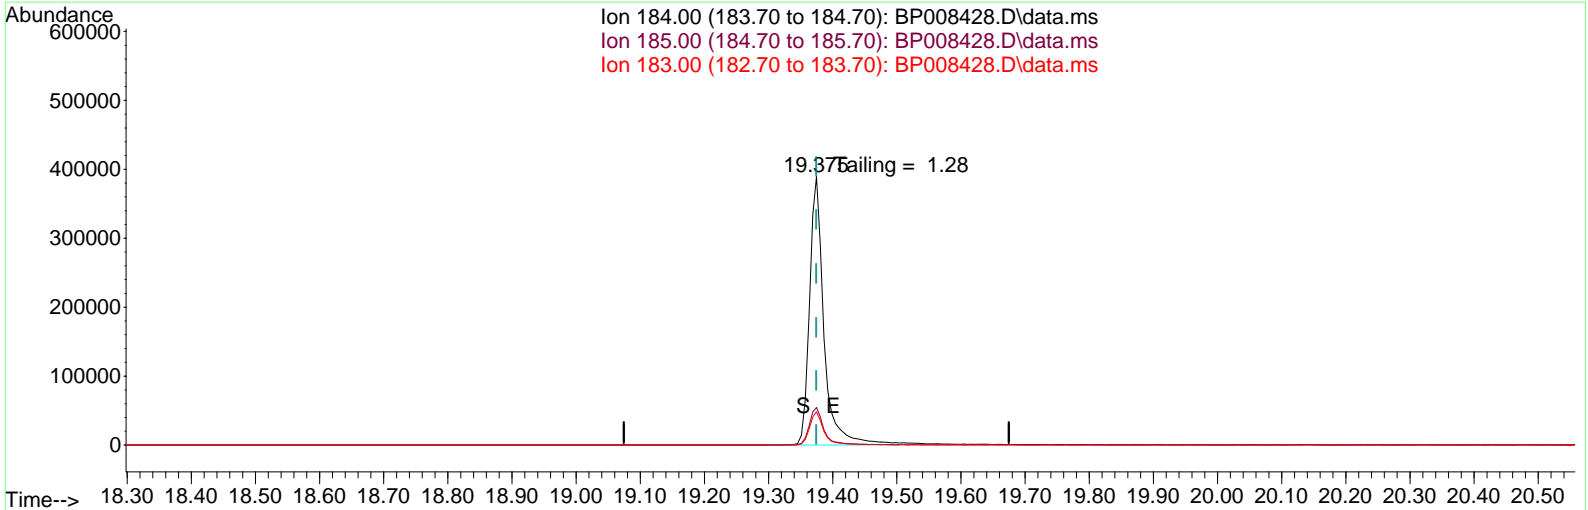

TIC: BP008428.D\data.ms

(77) Benzidine

19.375min (+ 0.000) 30208.92 ng




response 617750

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.01
183.00	11.40	12.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121521\
 Data File : BP008428.D
 Acq On : 15 Dec 2021 23:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 06:44:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

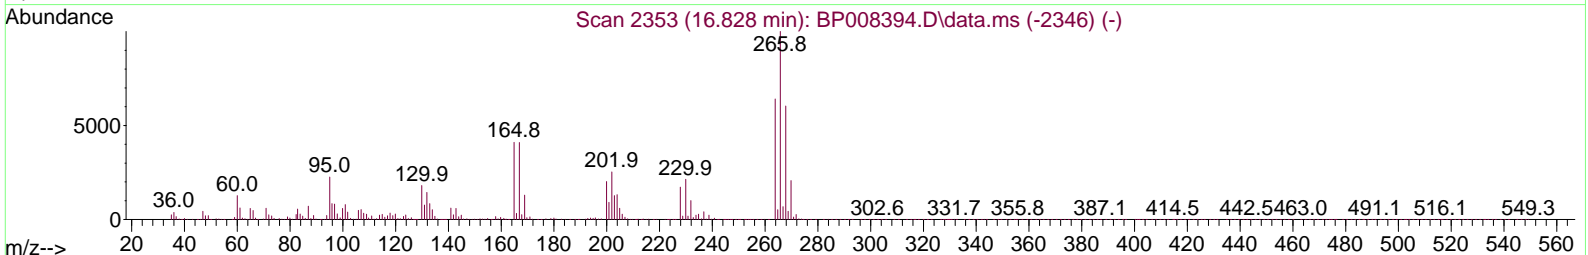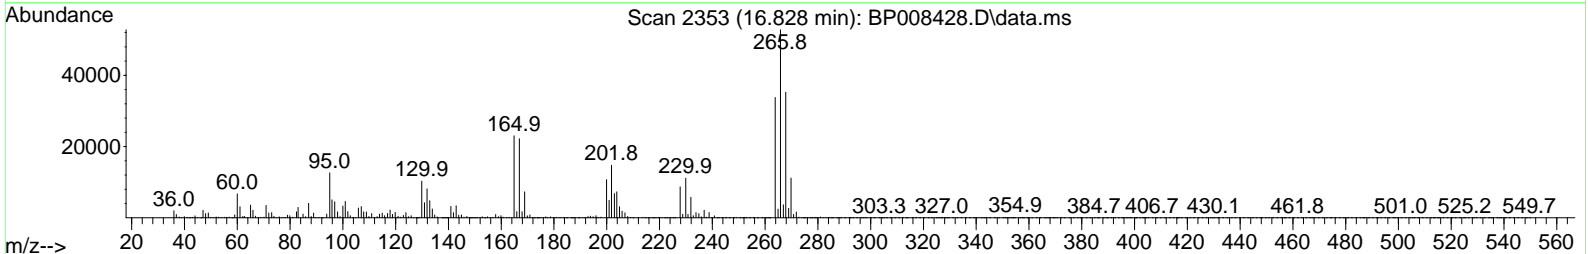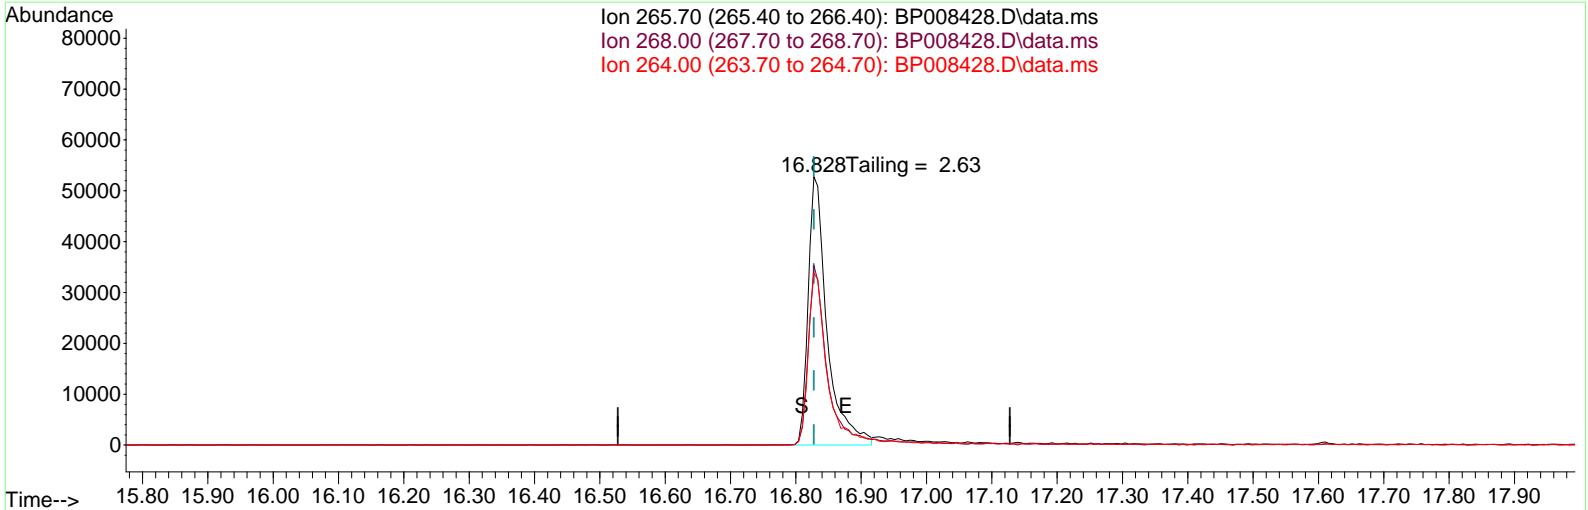

TIC: BP008428.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.000) 222676.66 ng

response 111343

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.84
264.00	61.90	63.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2021	BNA_P	BP008428.D
Compound Name	Response	Retention Time
DDT	61855	20.553
DDD	150996	20.139
DDE	930	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
151926	213781	71.07

Instrument :
 BNA_P
 ClientSampled :
 DFTPP