


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121522\
 Data File : BP013111.D
 Acq On : 15 Dec 2022 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 13 03:29:24 2022

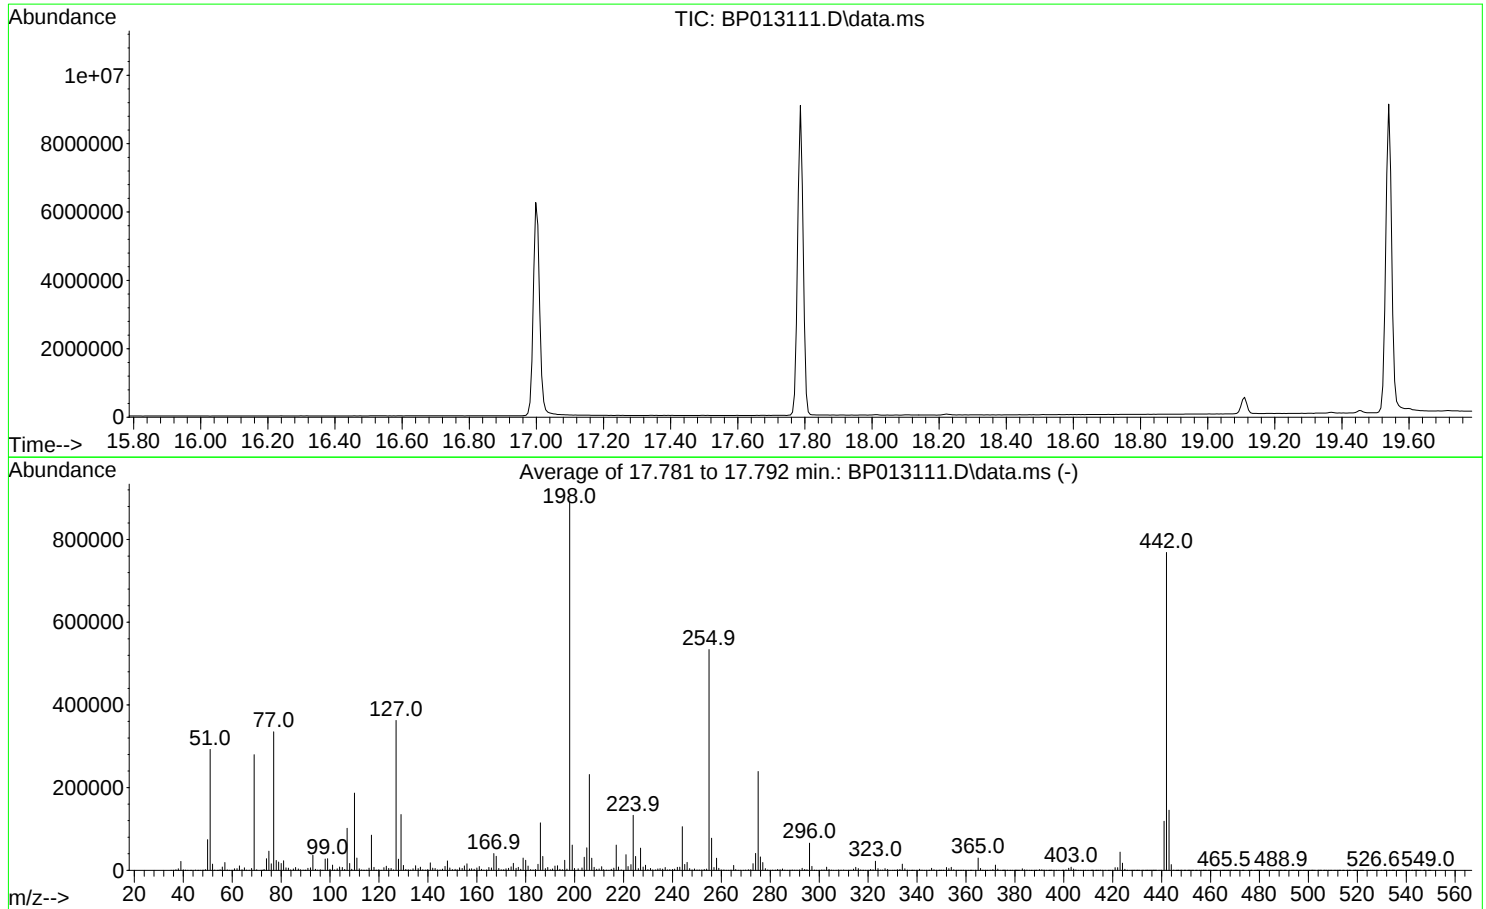




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	292237	PASS
68	69	0.00	2	1.6	4608	PASS
69	198	0.00	100	31.4	279816	PASS
70	69	0.00	2	0.6	1540	PASS
127	198	10	80	40.8	362621	PASS
197	198	0.00	2	0.3	2768	PASS
198	198	100	100	100.0	889776	PASS
199	198	5	9	6.8	60881	PASS
275	198	10	60	26.9	238976	PASS
365	198	1	100	3.3	29717	PASS
441	198	0.01	100	13.4	118847	PASS
442	442	100	100	100.0	768768	PASS
443	442	15	24	18.9	145243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121522\
Data File : BP013111.D
Acq On : 15 Dec 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 15 15:07:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

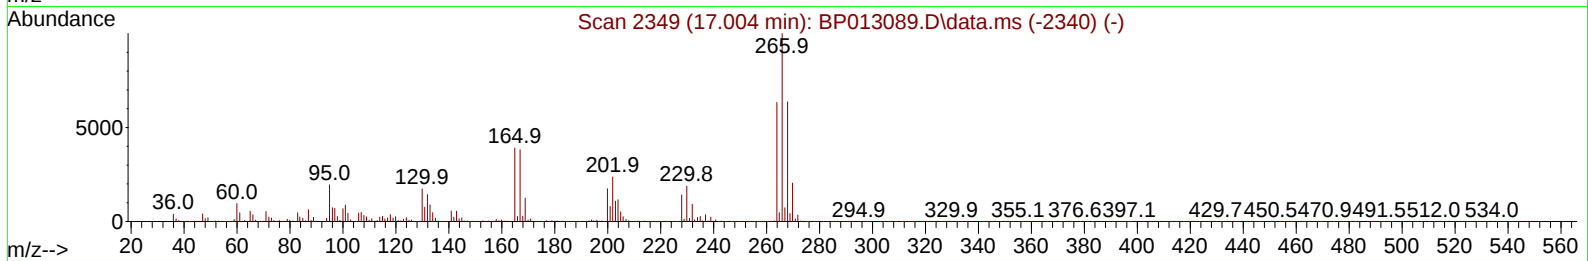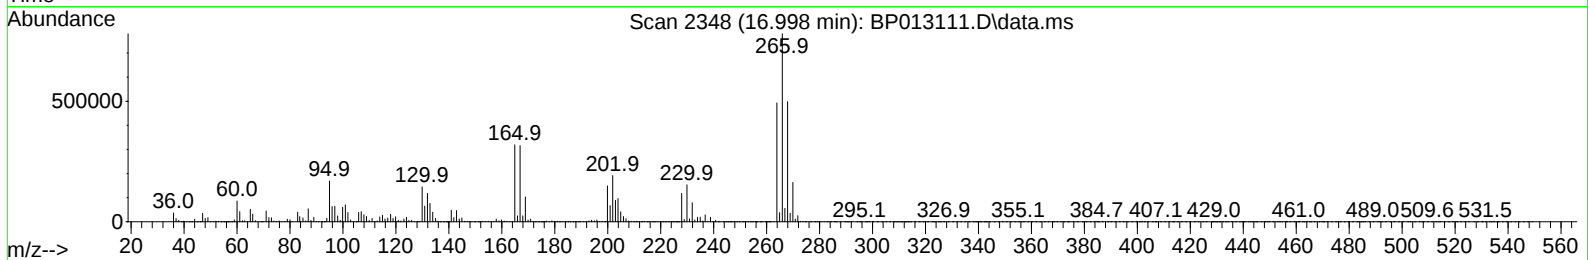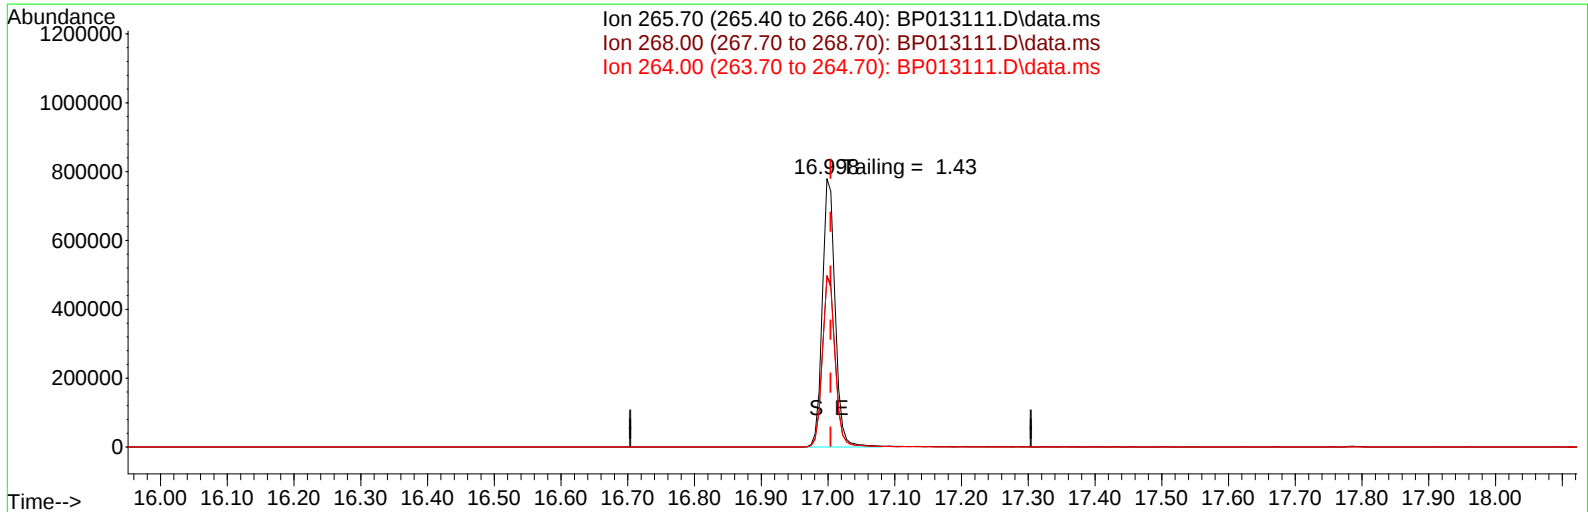

TIC: BP013111.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.006) 99991.19 ng




response 1046012

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.88
264.00	63.30	63.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121522\
Data File : BP013111.D
Acq On : 15 Dec 2022 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 15 15:07:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

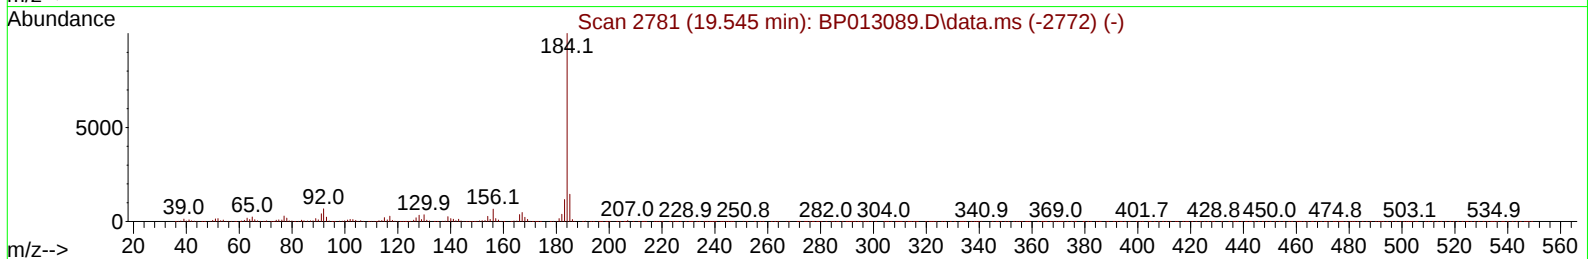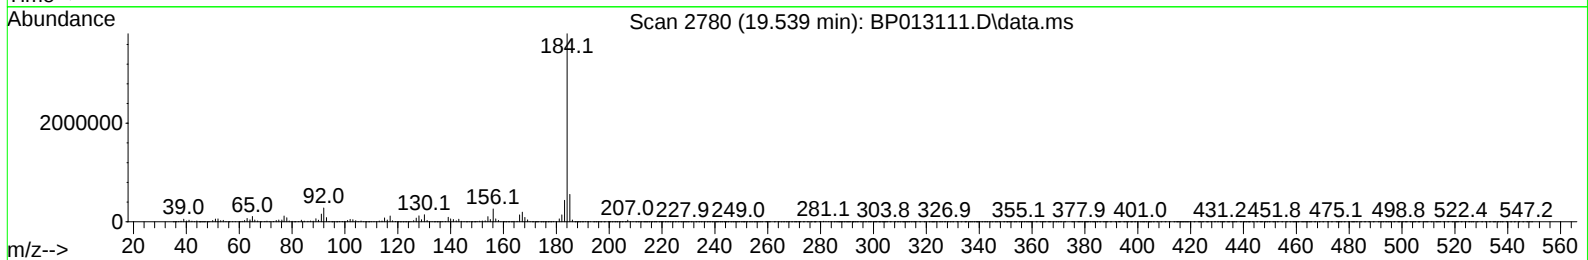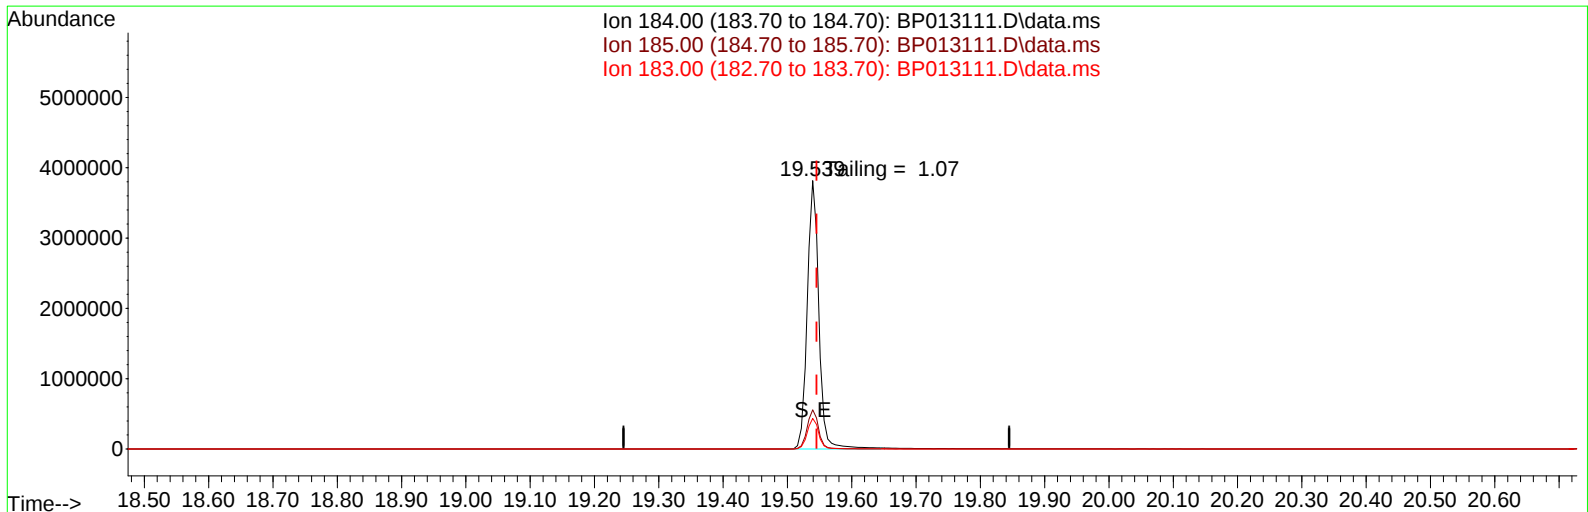

TIC: BP013111.D\data.ms

(77) Benzidine

19.539min (-0.006) 183249.69 ng

response 4841385

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.60
183.00	11.70	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2022	BNA_P	<u>BP013111.D</u>
Compound Name	Response	Retention Time
DDT	2377959	20.739
DDD	24697	20.363
DDE	807	19.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25504	2403463	1.06

Instrument :
BNA_P
ClientSampleId :
DFTPP