
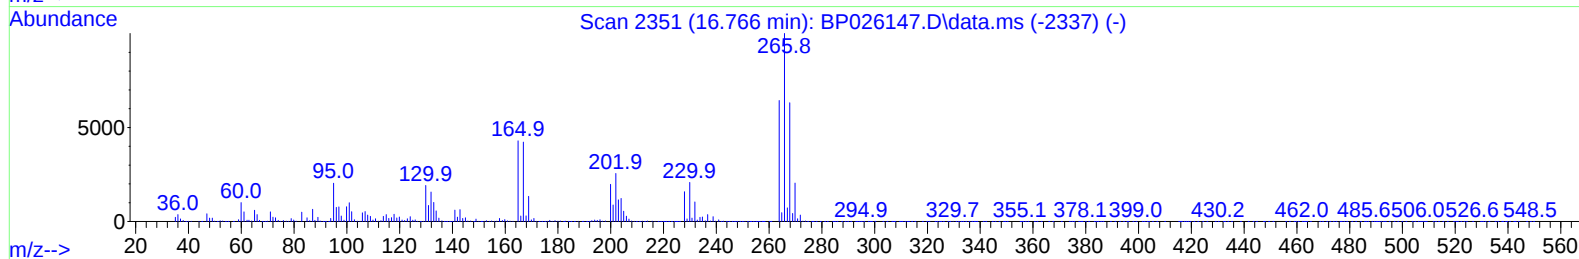
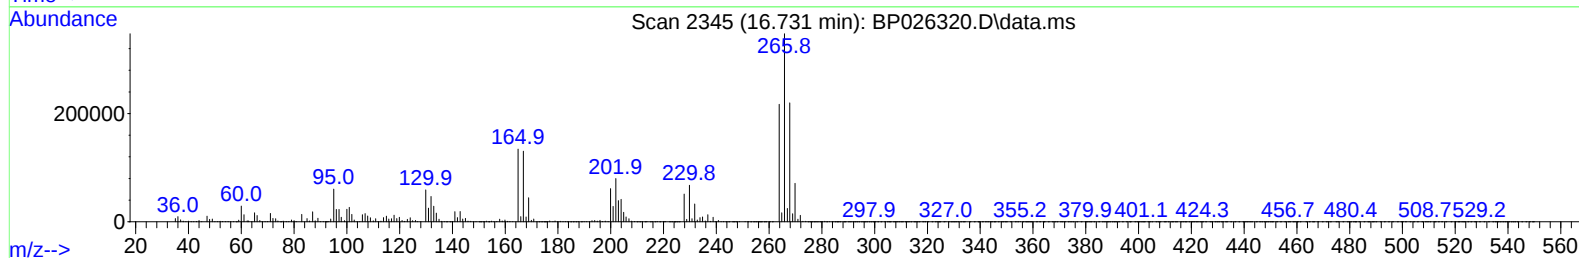


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121525\
Data File : BP026320.D
Acq On : 15 Dec 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:12:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 15 01:38:31 2025
Response via : Initial Calibration

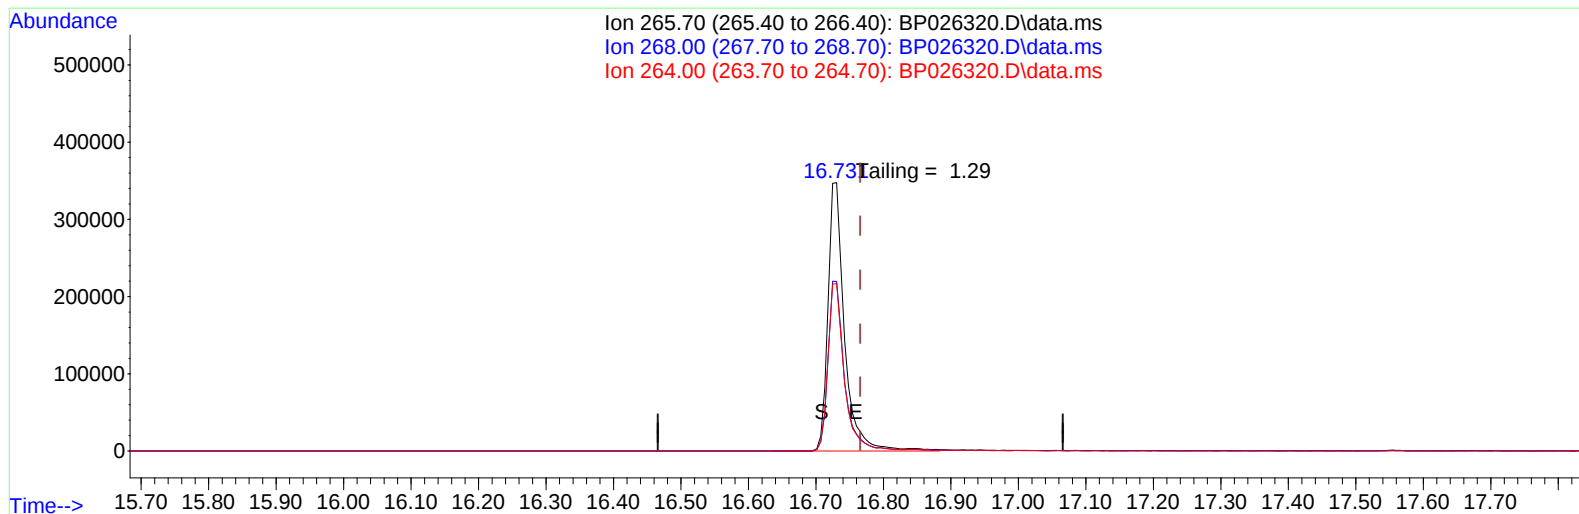

TIC: BP026320.D\data.ms

(70) Pentachlorophenol (C)




16.731min (-0.035) 1822810.57 ng

response 586542

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.23
264.00	62.70	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121525\
Data File : BP026320.D
Acq On : 15 Dec 2025 10:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 11:12:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 15 01:38:31 2025
Response via : Initial Calibration

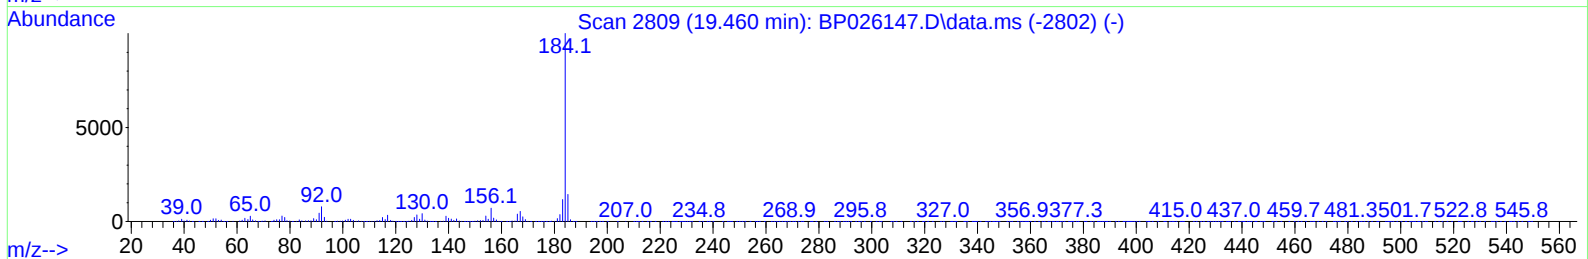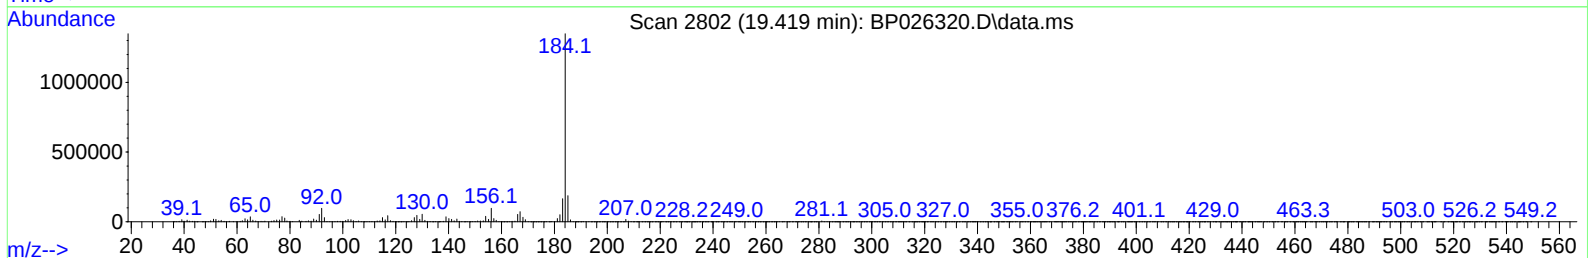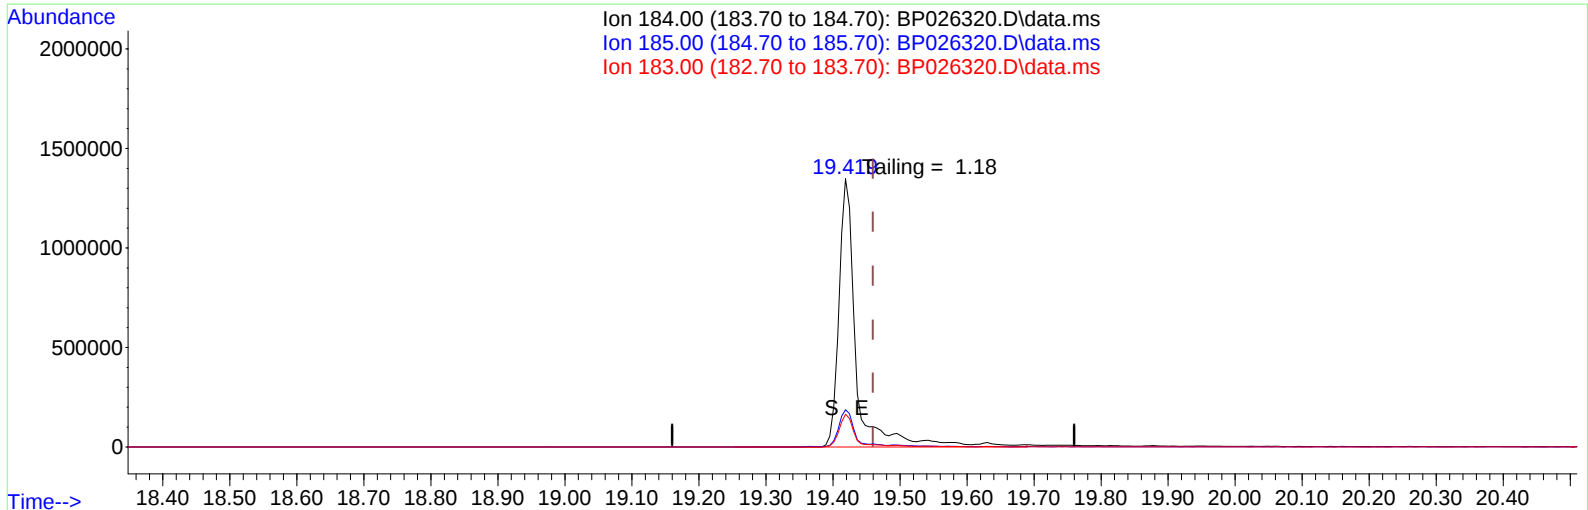

TIC: BP026320.D\data.ms

(77) Benzidine

19.419min (-0.041) 245766.07 ng

response 2168247

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.90
183.00	11.30	12.23
0.00	0.00	0.00