

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121525\
 Data File : BP026325.D
 Acq On : 15 Dec 2025 14:50
 Operator : RC/JU
 Sample : Q3839-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AM7

Quant Time: Dec 15 15:25:49 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 15 14:15:35 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.649	152	234076	20.000	ng	0.00
21) Naphthalene-d8	10.413	136	872699	20.000	ng	0.00
39) Acenaphthene-d10	14.272	164	555224	20.000	ng	0.00
64) Phenanthrene-d10	17.084	188	1117393	20.000	ng	0.00
76) Chrysene-d12	21.530	240	1315558	20.000	ng	0.00
86) Perylene-d12	24.824	264	1478204	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.278	112	642507	44.130	ng	0.00
7) Phenol-d6	6.837	99	450804	24.525	ng	0.00
23) Nitrobenzene-d5	8.790	82	1042447	67.629	ng	0.00
42) 2,4,6-Tribromophenol	15.795	330	969348	131.371	ng	0.00
45) 2-Fluorobiphenyl	12.878	172	2741542	71.387	ng	-0.01
79) Terphenyl-d14	19.831	244	5320486	80.578	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121525\
Data File : BP026325.D
Acq On : 15 Dec 2025 14:50
Operator : RC/JU
Sample : Q3839-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AM7

Quant Time: Dec 15 15:25:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 15 14:15:35 2025
Response via : Initial Calibration




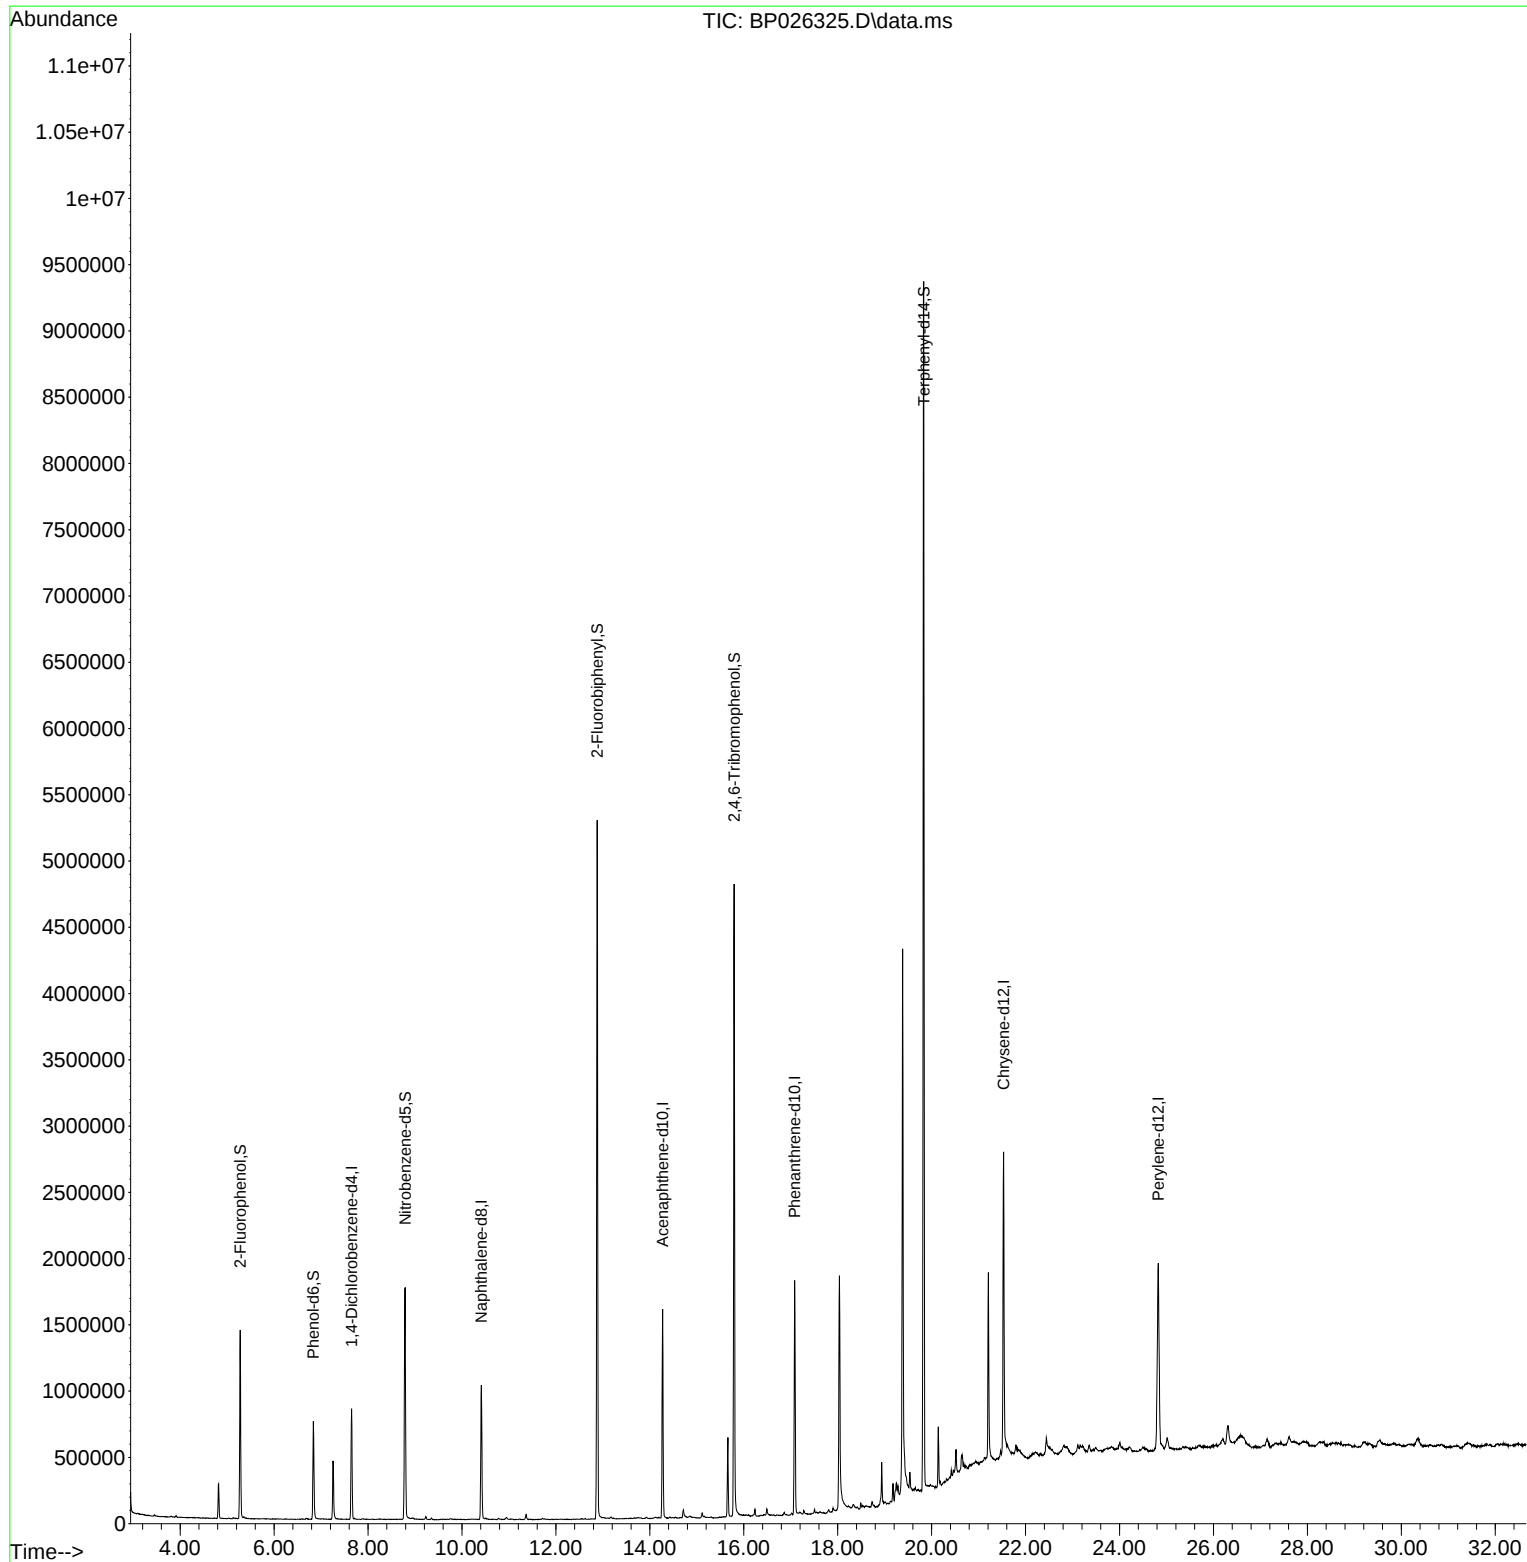




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.649 min Scan# 80
Delta R.T. -0.006 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50




Instrument :
BNA_P
ClientSampleId :
C0AM7


Tgt Ion:152 Resp: 234076
Ion Ratio Lower Upper
152 100
150 154.1 123.0 184.6
115 58.2 46.3 69.5

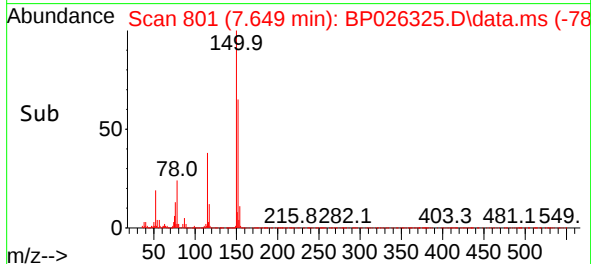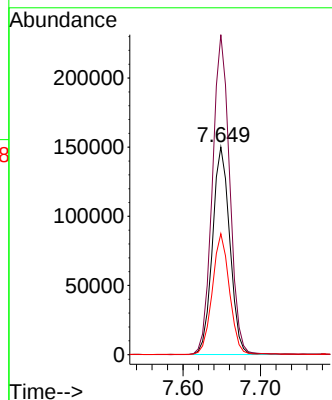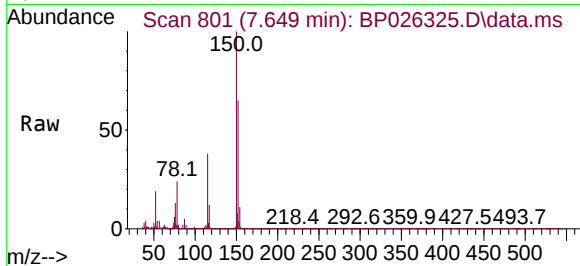

#5
2-Fluorophenol
Concen: 44.130 ng
RT: 5.278 min Scan# 398
Delta R.T. 0.000 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50

Tgt Ion:112 Resp: 642507
Ion Ratio Lower Upper
112 100
64 54.5 45.8 68.6
63 28.6 23.5 35.3


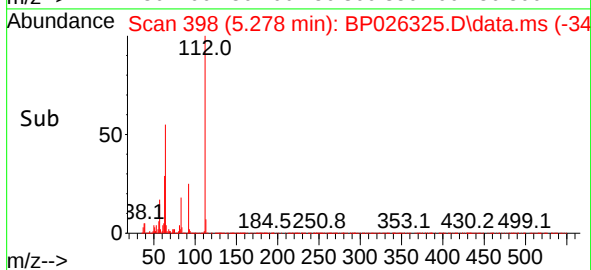
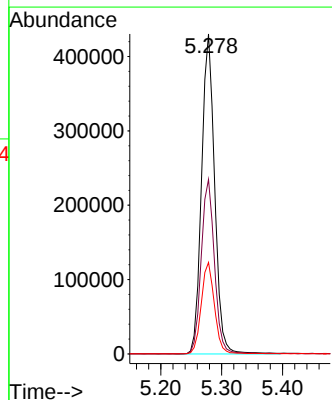
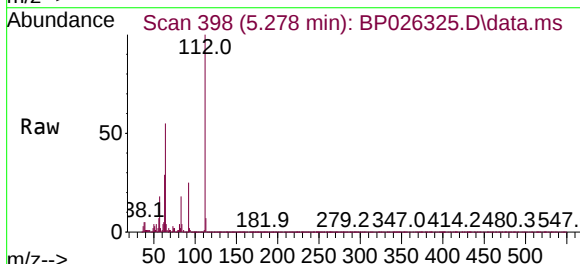




#7
Phenol-d6
Concen: 24.525 ng
RT: 6.837 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50




Instrument :
BNA_P
ClientSampleId :
COAM7

Tgt Ion:	99	Resp:	450804
Ion	Ratio	Lower	Upper
99	100		
42	16.4	12.9	19.3
71	33.1	24.8	37.2

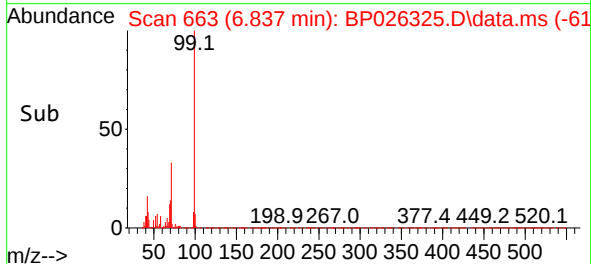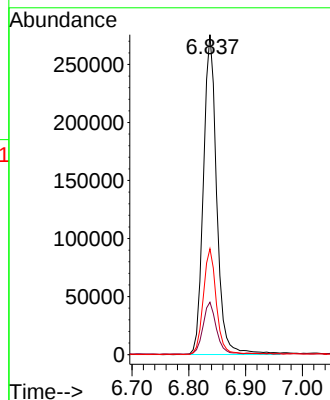

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.413 min Scan# 1271
Delta R.T. 0.006 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50

Tgt Ion:	136	Resp:	872699
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.7	13.1
54	7.8	6.4	9.6
68	5.5	4.9	7.3


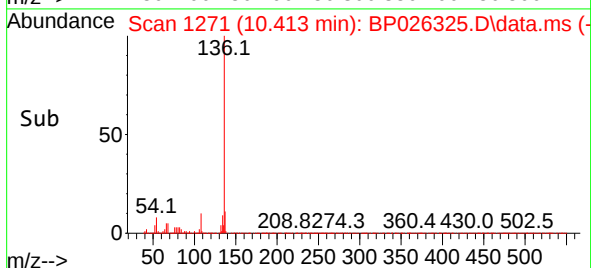
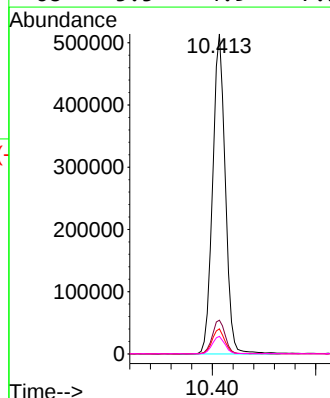
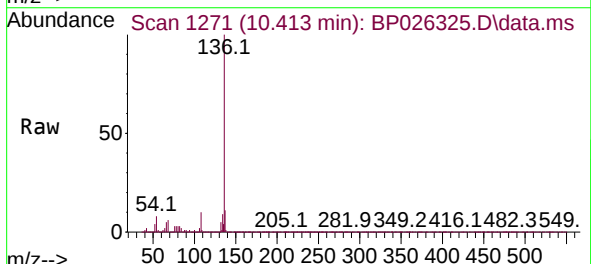




#23
Nitrobenzene-d5
Concen: 67.629 ng
RT: 8.790 min Scan# 999
Delta R.T. 0.000 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50




Instrument :
BNA_P
ClientSampleId :
COAM7


Tgt Ion: 82 Resp: 1042447
Ion Ratio Lower Upper
82 100
128 48.3 37.4 56.0
54 49.1 41.6 62.4

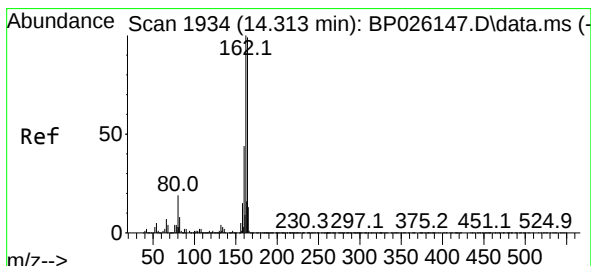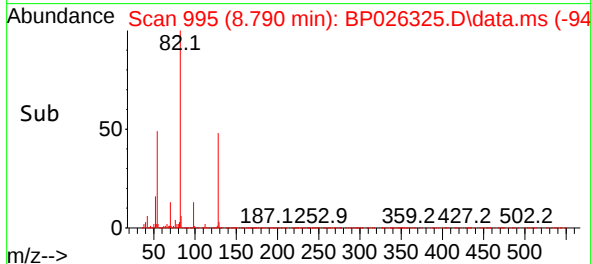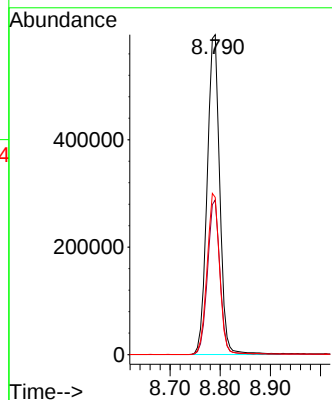

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.272 min Scan# 1927
Delta R.T. -0.006 min
Lab File: BP026325.D
Acq: 15 Dec 2025 14:50

Tgt Ion:164 Resp: 555224
Ion Ratio Lower Upper
164 100
162 99.8 80.3 120.5
160 43.2 35.2 52.8

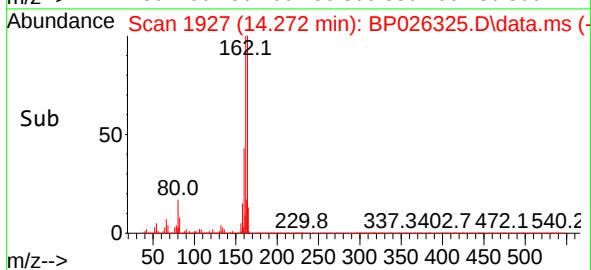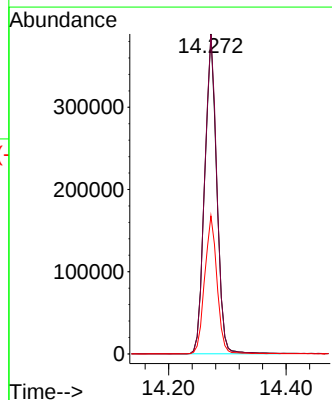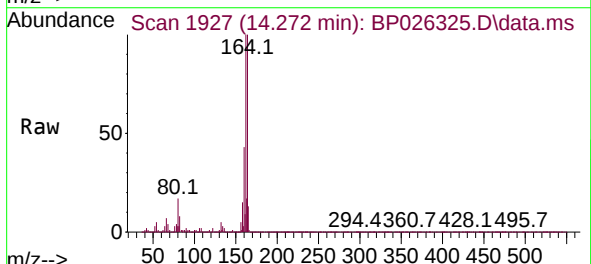

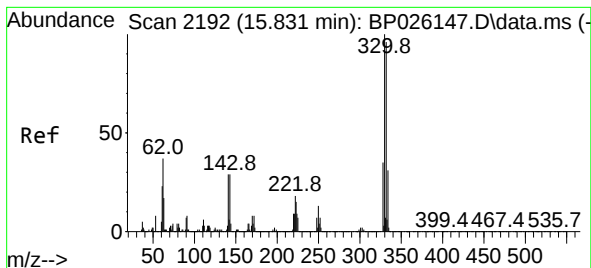

#42

2,4,6-Tribromophenol

Concen: 131.371 ng

RT: 15.795 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50

Instrument :

BNA_P

ClientSampleId :

COAM7





Tgt Ion:330 Resp: 969348

Ion Ratio Lower Upper

330 100

332 96.7 78.0 117.0

141 30.2 26.8 40.2

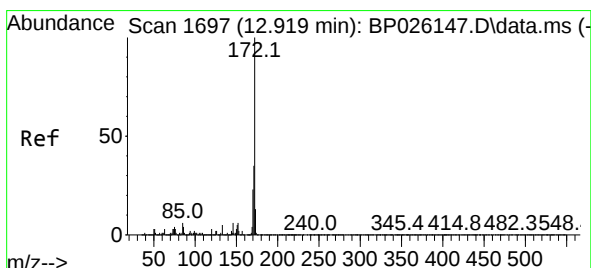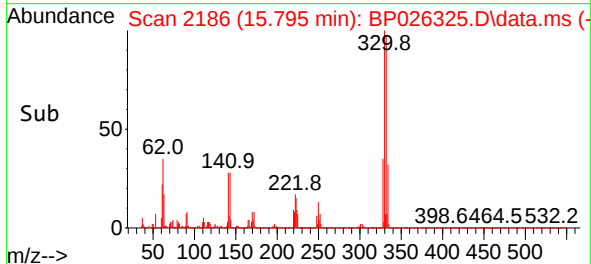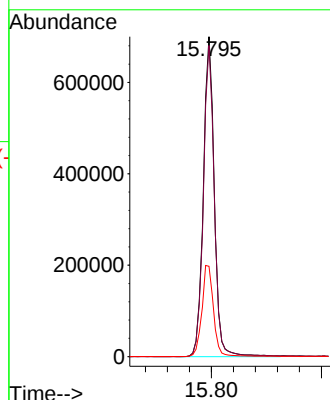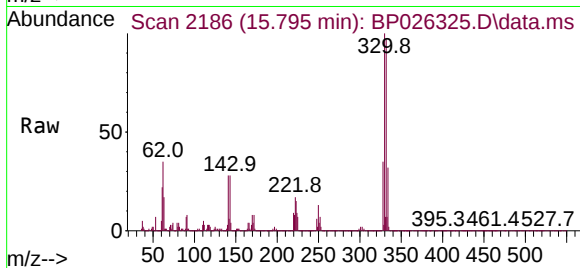

#45

2-Fluorobiphenyl

Concen: 71.387 ng

RT: 12.878 min Scan# 1690

Delta R.T. -0.012 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50




Tgt Ion:172 Resp: 2741542


Ion Ratio Lower Upper

172 100

171 35.1 28.2 42.4

170 23.3 18.7 28.1

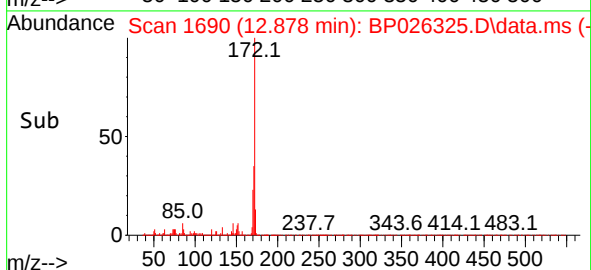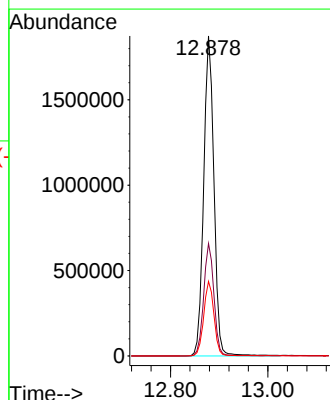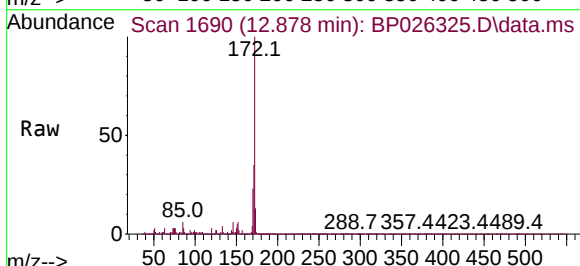

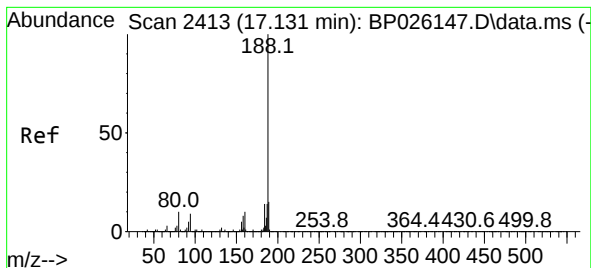

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.084 min Scan# 2413

Delta R.T. 0.000 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50

Instrument :

BNA_P

ClientSampleId :

C0AM7





Tgt Ion:188 Resp: 1117393

Ion Ratio Lower Upper

188 100

94 8.4 7.8 11.6

80 9.5 8.2 12.2

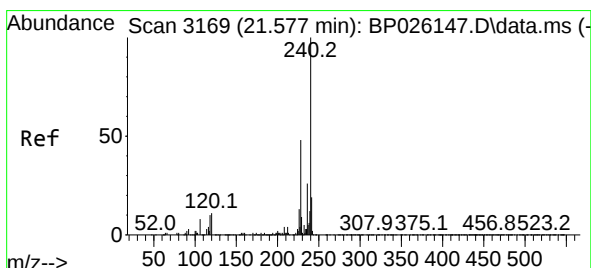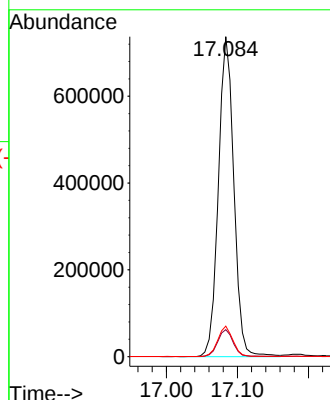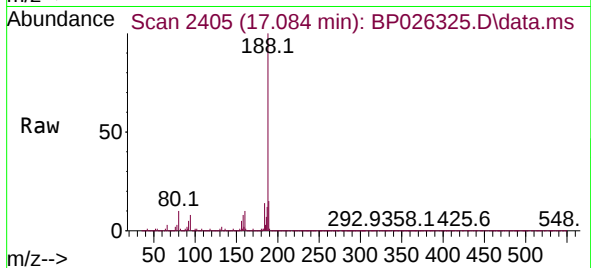

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.530 min Scan# 3161

Delta R.T. -0.006 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50




Tgt Ion:240 Resp: 1315558


Ion Ratio Lower Upper

240 100

120 9.6 9.0 13.4

236 26.3 20.4 30.6

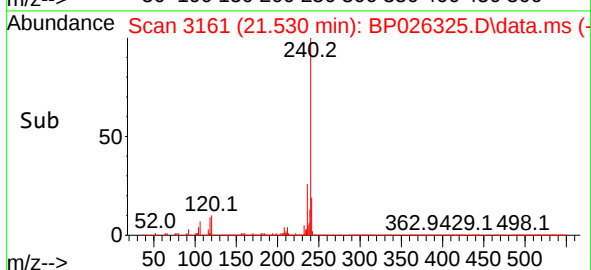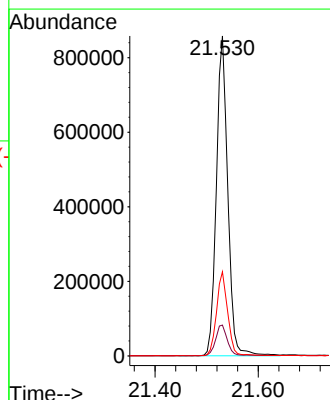

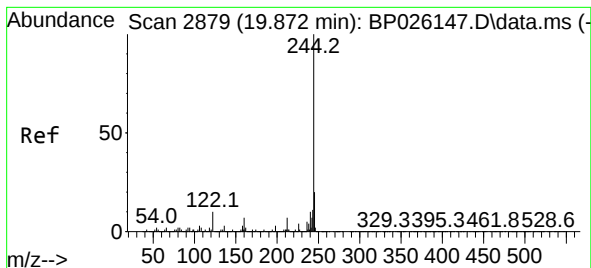

#79

Terphenyl-d14

Concen: 80.578 ng

RT: 19.831 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50

Instrument :

BNA_P

ClientSampleId :

COAM7





Tgt Ion:244 Resp: 5320486

Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.8

122 8.8 8.2 12.2

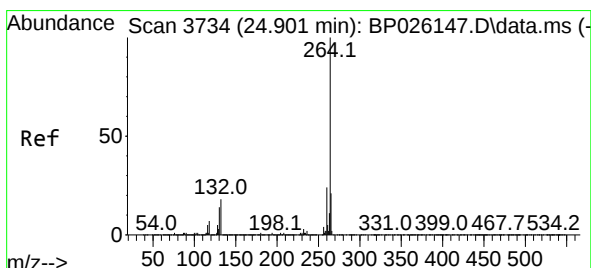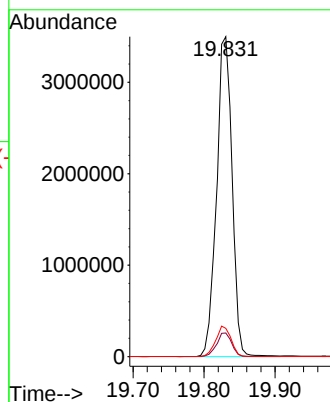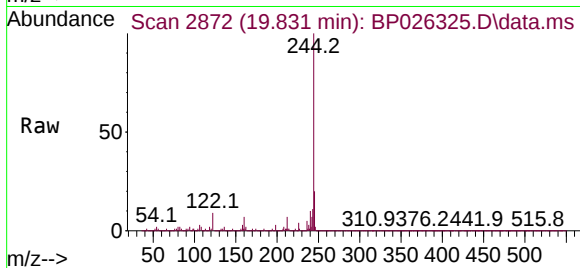

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.824 min Scan# 3721

Delta R.T. -0.012 min

Lab File: BP026325.D

Acq: 15 Dec 2025 14:50

Tgt Ion:264 Resp: 1478204

Ion Ratio Lower Upper

264 100

260 23.8 18.7 28.1

265 22.5 17.5 26.3

