
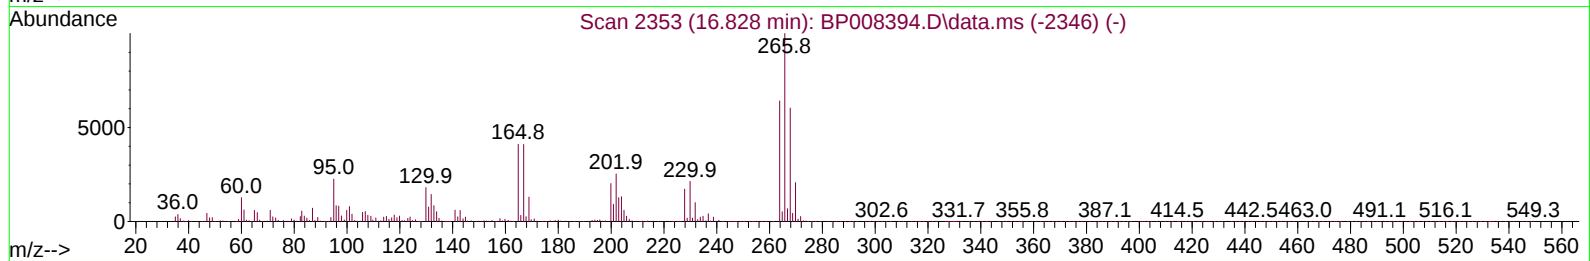
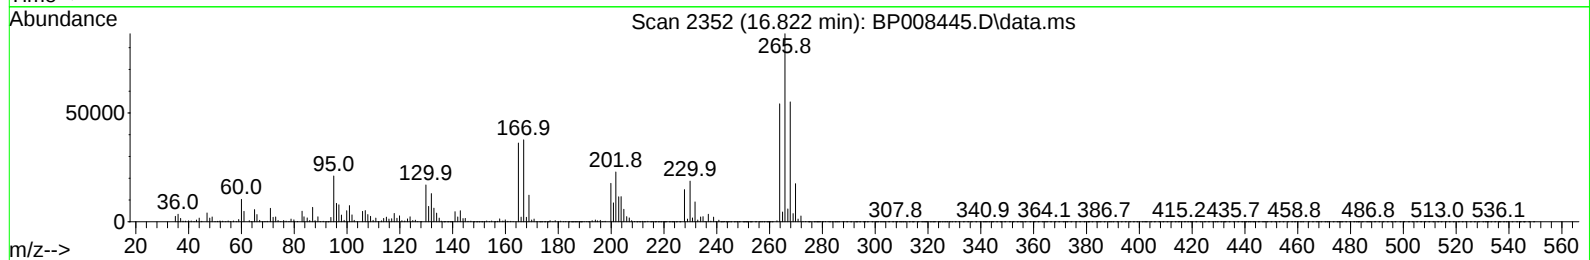


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008445.D
Acq On : 16 Dec 2021 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 14:21:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 17:59:47 2021
Response via : Initial Calibration

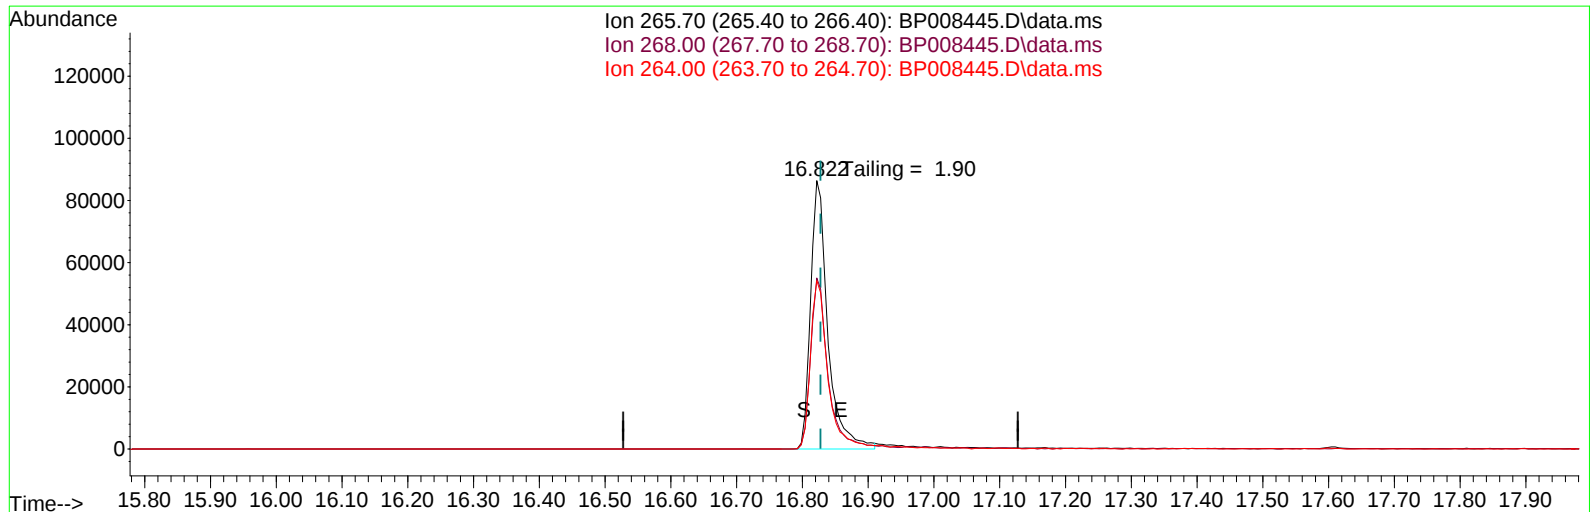

TIC: BP008445.D\data.ms

(70) Pentachlorophenol (C)




16.822min (-0.006) 733238.07 ng

response 159815

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.77
264.00	61.90	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
 Data File : BP008445.D
 Acq On : 16 Dec 2021 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 14:21:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

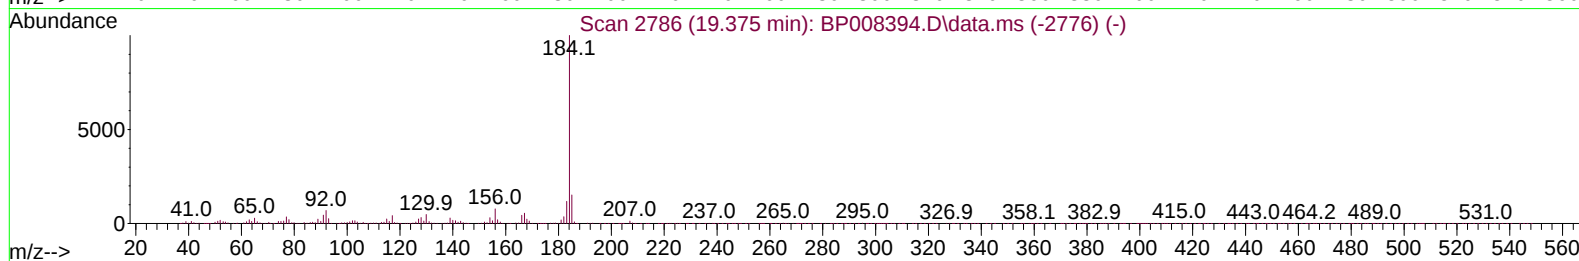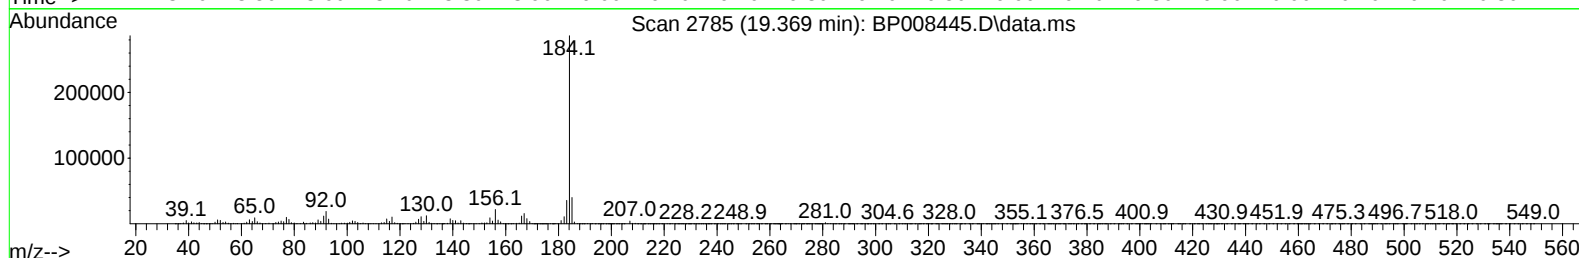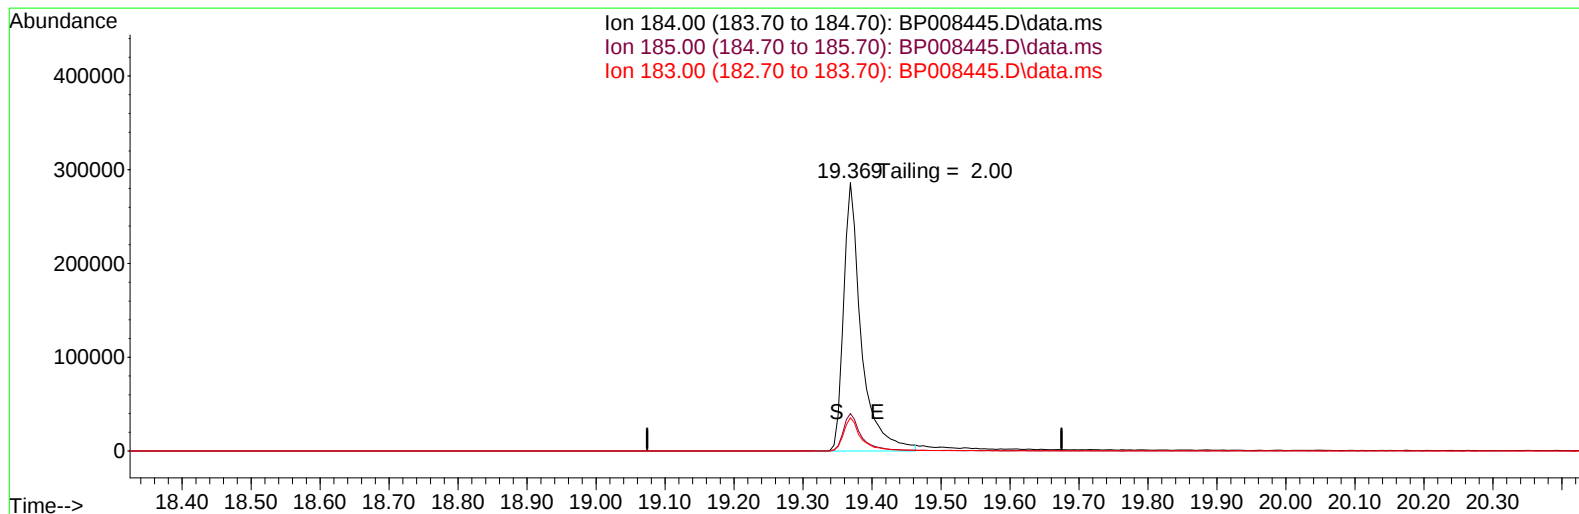

TIC: BP008445.D\data.ms

(77) Benzidine

19.369min (-0.006) 722466.90 ng m

response 512983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.99
183.00	11.40	12.44
0.00	0.00	0.00