

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
 Data File : BP008452.D
 Acq On : 16 Dec 2021 14:49
 Operator : CG/JU
 Sample : M5067-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BASE

Quant Time: Dec 16 15:51:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.734	152	51559	20.000	ng	-0.01
21) Naphthalene-d8	10.528	136	178359	20.000	ng	-0.01
39) Acenaphthene-d10	14.392	164	111581	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	239074	20.000	ng	0.00
76) Chrysene-d12	21.269	240	275424	20.000	ng	# 0.00
86) Perylene-d12	23.639	264	331413	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	398191	121.965	ng	0.00
7) Phenol-d6	6.934	99	436868	99.632	ng	0.00
23) Nitrobenzene-d5	8.899	82	374179	88.877	ng	-0.01
42) 2,4,6-Tribromophenol	15.898	330	245149	149.502	ng	0.00
45) 2-Fluorobiphenyl	13.010	172	738371	84.120	ng	0.00
79) Terphenyl-d14	19.733	244	1331474	84.135	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.174	149	23314	2.308	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008452.D
Acq On : 16 Dec 2021 14:49
Operator : CG/JU
Sample : M5067-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BASE

Quant Time: Dec 16 15:51:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 17:59:47 2021
Response via : Initial Calibration




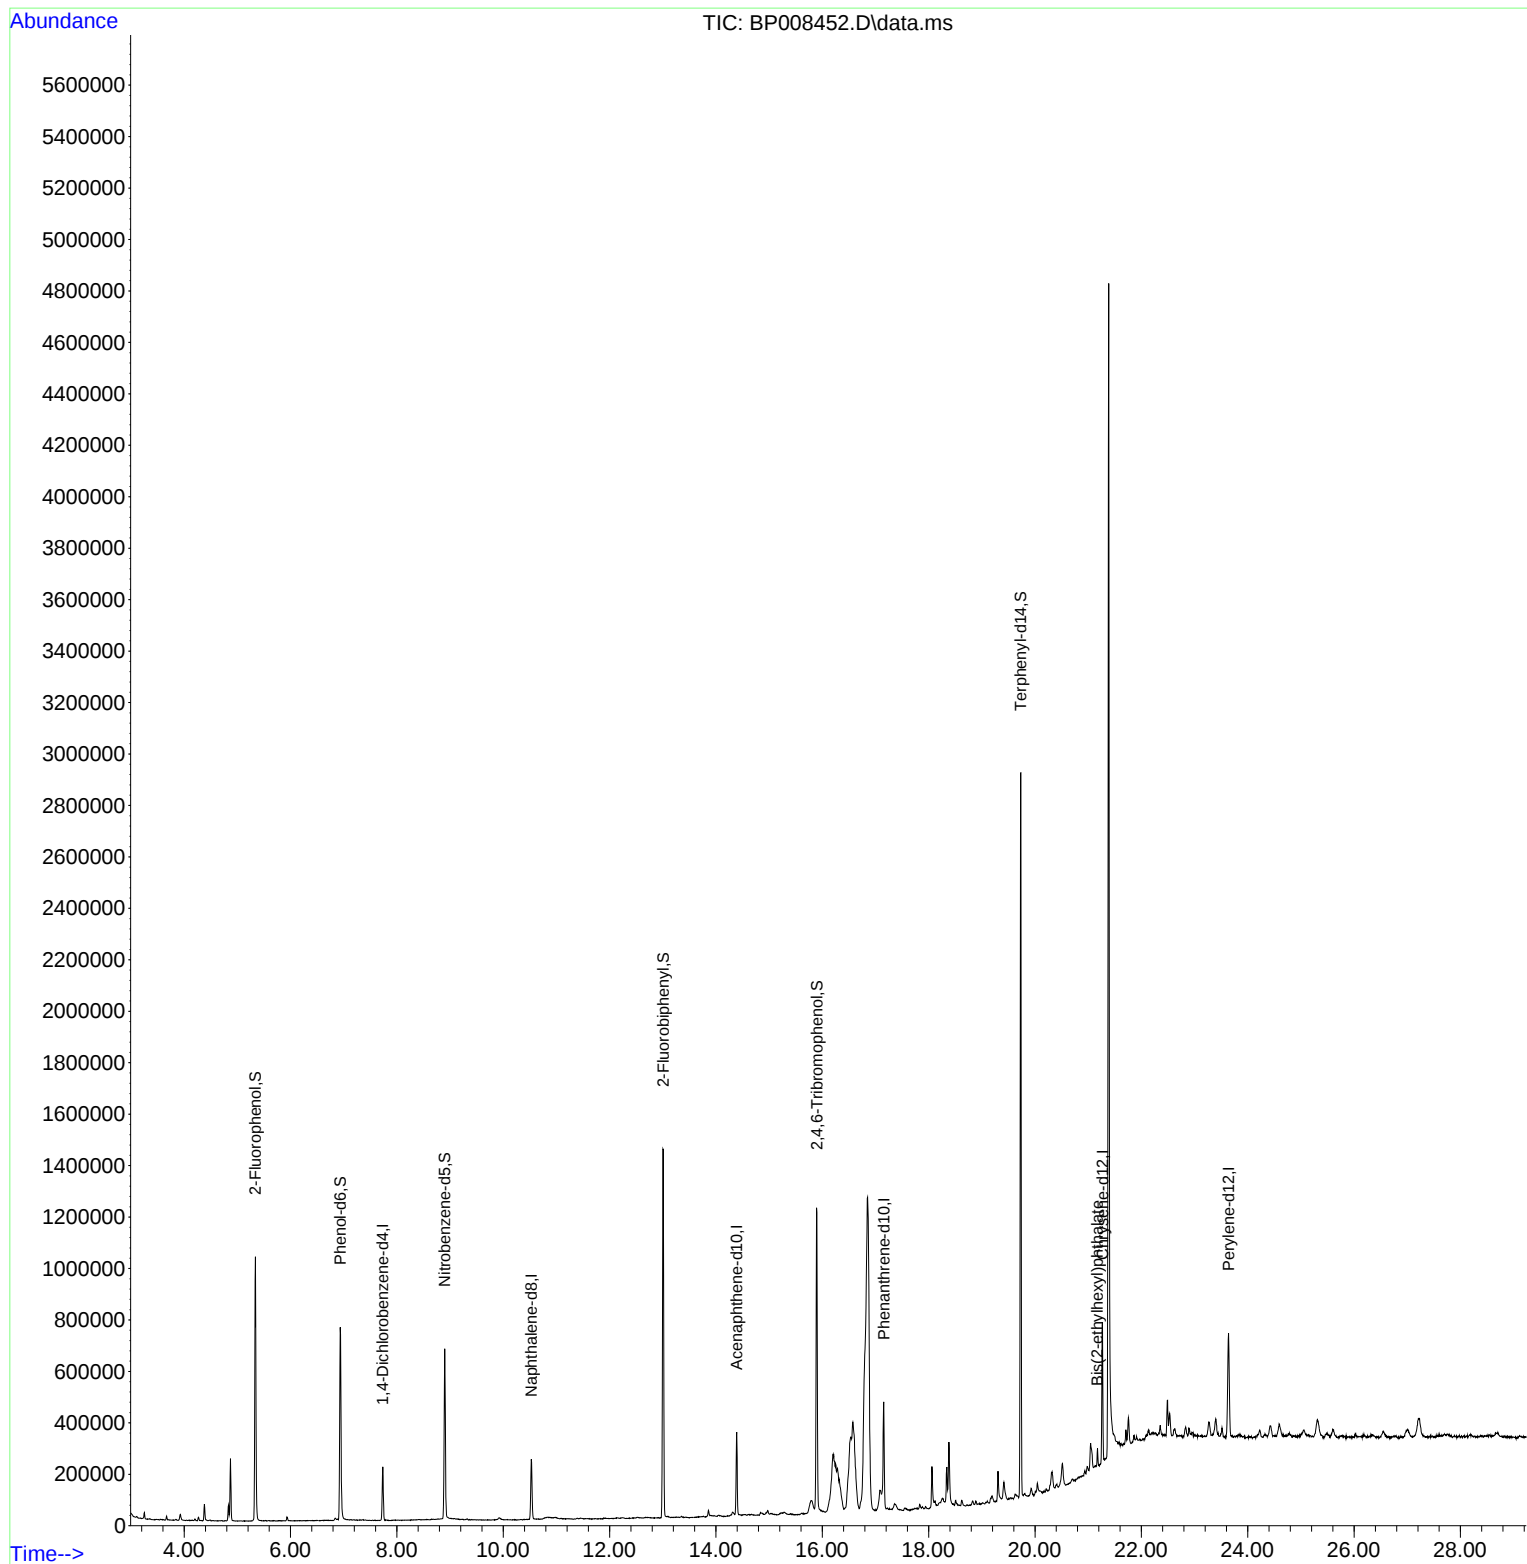




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.734 min Scan# 80
Delta R.T. -0.012 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49




Instrument :
BNA_P
ClientSampleId :
BASE


Tgt Ion:152 Resp: 51559
Ion Ratio Lower Upper
152 100
150 160.9 125.7 188.5
115 70.2 50.7 76.1

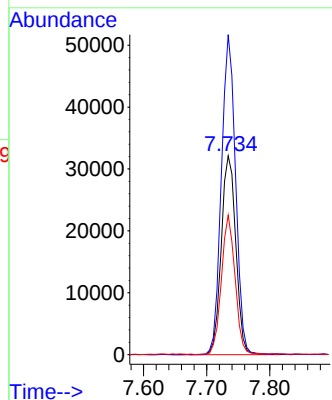

#5
2-Fluorophenol
Concen: 121.965 ng
RT: 5.340 min Scan# 400
Delta R.T. -0.006 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49

Tgt Ion:112 Resp: 398191
Ion Ratio Lower Upper
112 100
64 66.9 53.4 80.2
63 34.2 27.8 41.8


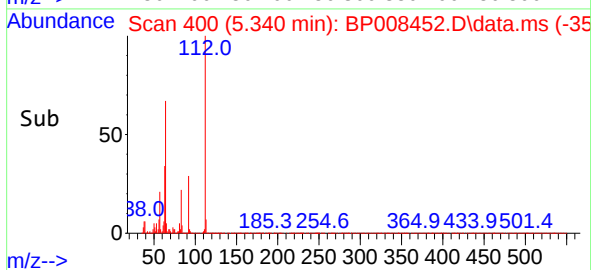
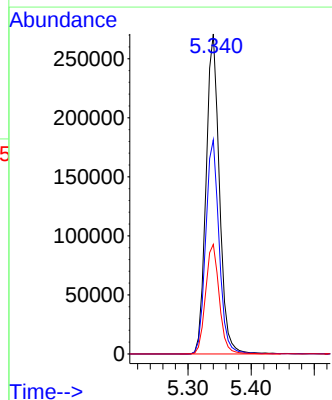



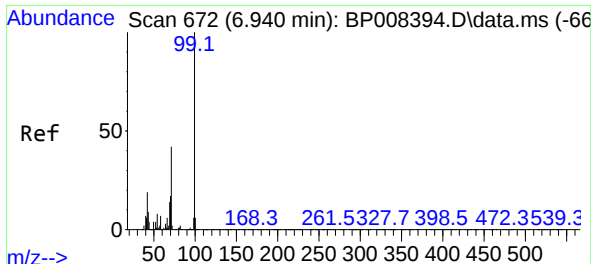

#7
Phenol-d6
Concen: 99.632 ng
RT: 6.934 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49




Instrument :
BNA_P
ClientSampleId :
BASE


Tgt Ion: 99 Resp: 436868
Ion Ratio Lower Upper
99 100
42 20.3 14.6 22.0
71 42.7 31.1 46.7

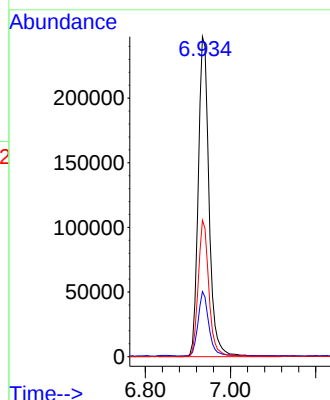

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.528 min Scan# 1282
Delta R.T. -0.012 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49

Tgt Ion: 136 Resp: 178359
Ion Ratio Lower Upper
136 100
137 10.6 9.0 13.6
54 10.7 8.2 12.4
68 7.0 5.8 8.8

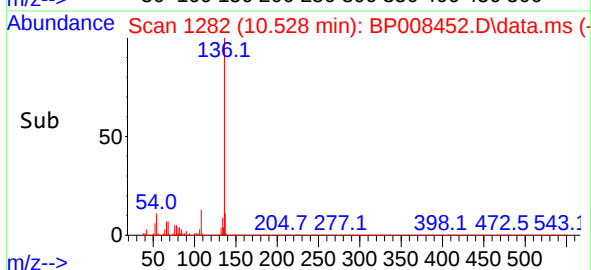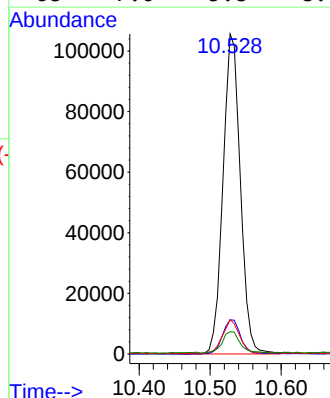



#23

Nitrobenzene-d5

Concen: 88.877 ng

RT: 8.899 min Scan# 1005

Delta R.T. -0.012 min

Lab File: BP008452.D

Acq: 16 Dec 2021 14:49

Instrument :

BNA_P

ClientSampleId :

BASE





Tgt Ion: 82 Resp: 374179

Ion Ratio Lower Upper

82 100

128 38.0 29.6 44.4

54 53.8 42.7 64.1

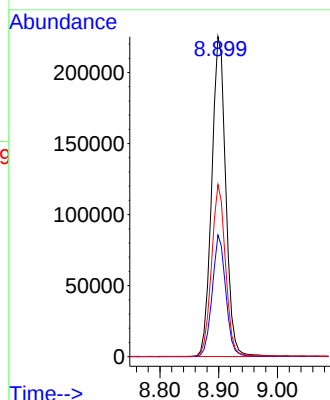

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.392 min Scan# 1939

Delta R.T. -0.006 min

Lab File: BP008452.D

Acq: 16 Dec 2021 14:49




Tgt Ion: 164 Resp: 111581


Ion Ratio Lower Upper

164 100

162 104.3 81.9 122.9

160 47.0 35.4 53.0


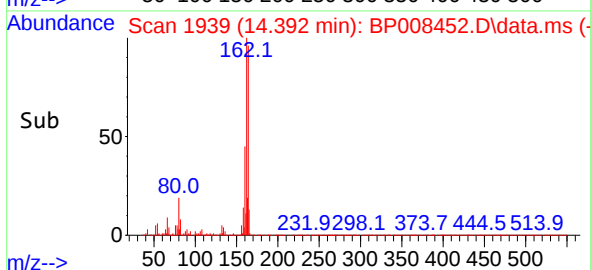
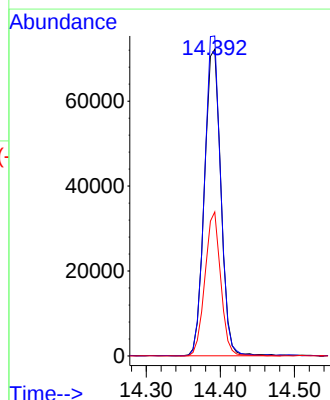





#42
2,4,6-Tribromophenol
Concen: 149.502 ng
RT: 15.898 min Scan# 2195
Delta R.T. -0.006 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49




Instrument :
BNA_P
ClientSampleId :
BASE


Tgt Ion:330 Resp: 245149
Ion Ratio Lower Upper
330 100
332 96.2 77.0 115.4
141 30.6 28.4 42.6

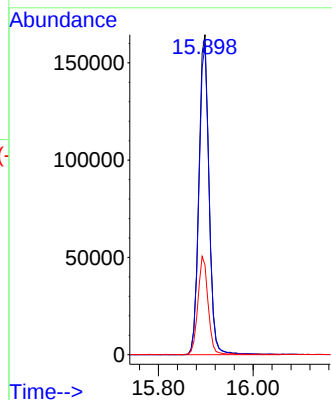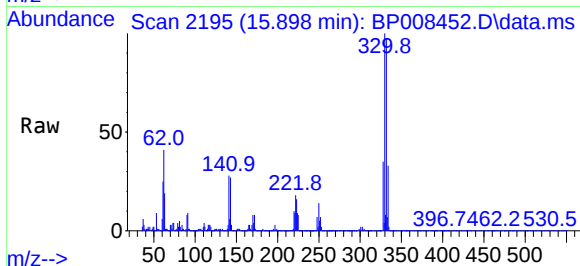

#45
2-Fluorobiphenyl
Concen: 84.120 ng
RT: 13.010 min Scan# 1704
Delta R.T. -0.006 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49

Tgt Ion:172 Resp: 738371
Ion Ratio Lower Upper
172 100
171 36.0 28.0 42.0
170 23.6 18.9 28.3


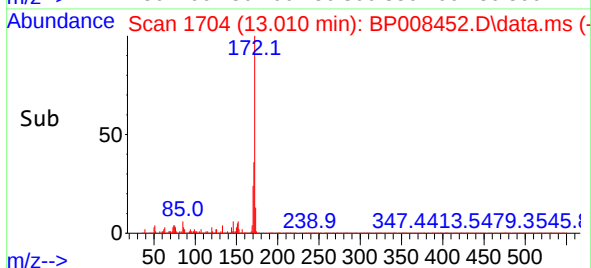
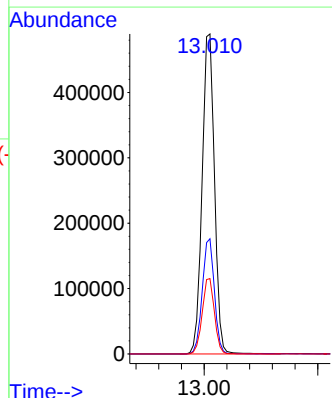
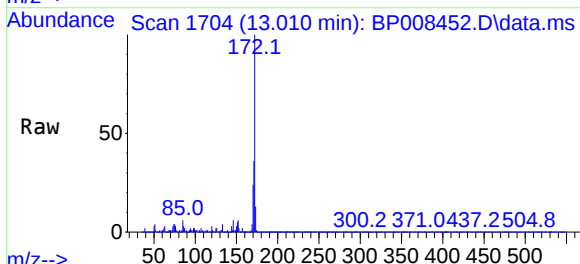




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.157 min Scan# 2410
Delta R.T. -0.006 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49




Instrument :
BNA_P
ClientSampleId :
BASE


Tgt Ion:188 Resp: 239074
Ion Ratio Lower Upper
188 100
94 8.0 7.2 10.8
80 8.9 8.2 12.4

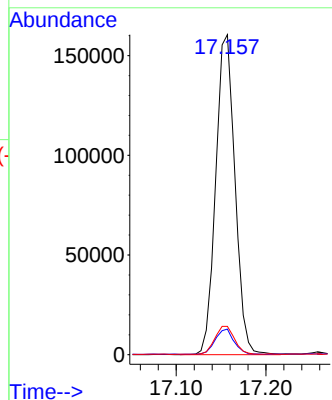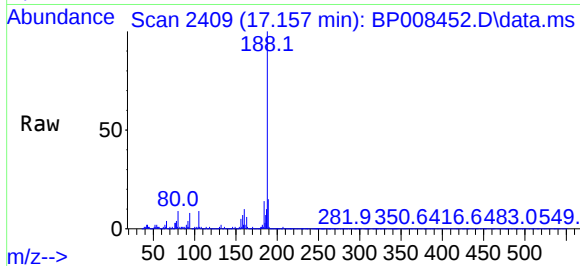

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.269 min Scan# 3108
Delta R.T. 0.000 min
Lab File: BP008452.D
Acq: 16 Dec 2021 14:49

Tgt Ion:240 Resp: 275424
Ion Ratio Lower Upper
240 100
120 7.0 7.3 10.9#
236 26.9 21.4 32.2


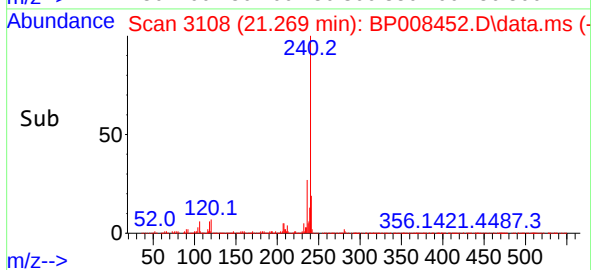
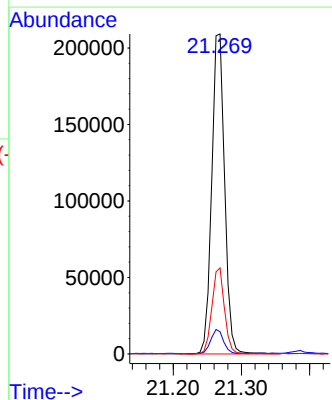
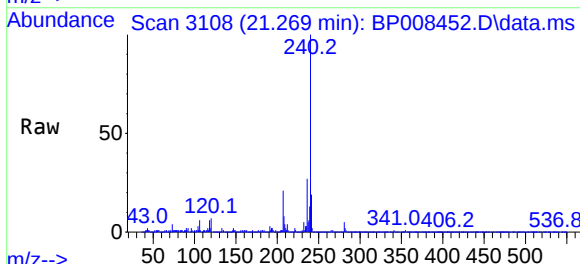




#79
 Terphenyl-d14
 Concen: 84.135 ng
 RT: 19.733 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BP008452.D
 Acq: 16 Dec 2021 14:49




Instrument :
 BNA_P
 ClientSampleId :
 BASE


Tgt Ion:244 Resp: 1331474
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 6.8 6.6 9.8

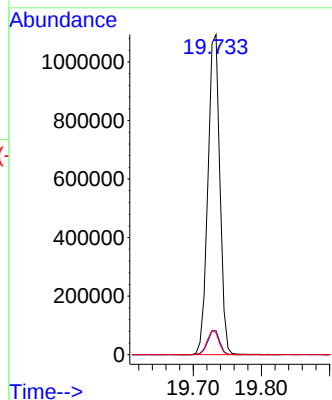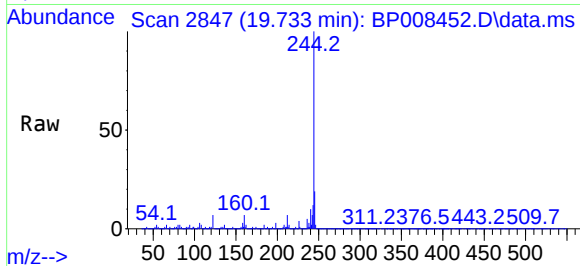

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.308 ng
 RT: 21.174 min Scan# 3092
 Delta R.T. -0.006 min
 Lab File: BP008452.D
 Acq: 16 Dec 2021 14:49

Tgt Ion:149 Resp: 23314
 Ion Ratio Lower Upper
 149 100
 167 28.6 22.5 33.7
 279 5.5 3.5 5.3#

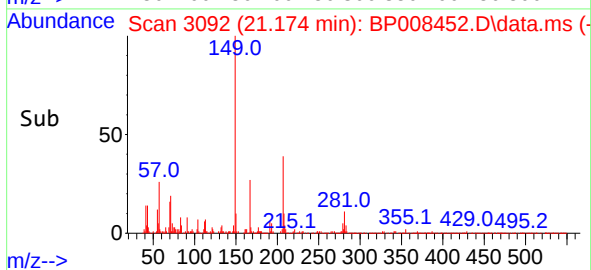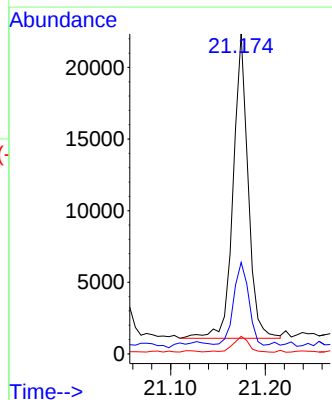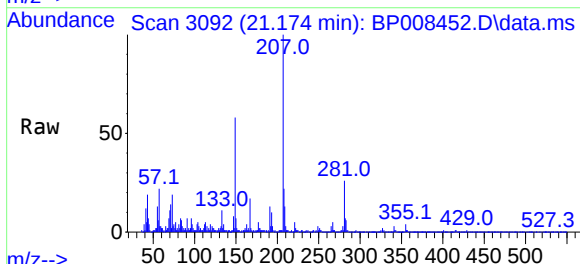

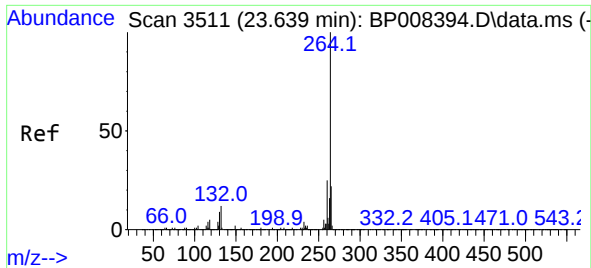

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.639 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP008452.D
 Acq: 16 Dec 2021 14:49

Instrument :
 BNA_P
 ClientSampleId :
 BASE

Tgt Ion:264 Resp: 331413
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.4 29.2
 265 22.7 17.6 26.4

