

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
 Data File : BP008447.D
 Acq On : 16 Dec 2021 11:45
 Operator : CG/JU
 Sample : PB141458BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141458BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	393	399	420	rBV	1438807	2268272	51.32%	11.704%
2	6.934	664	671	693	rBV	1276804	2201060	49.80%	11.358%
3	7.734	801	807	815	rBV	257057	401619	9.09%	2.072%
4	8.904	998	1006	1033	rBV	794584	1464737	33.14%	7.558%
5	10.534	1274	1283	1298	rBV	264767	501754	11.35%	2.589%
6	13.010	1697	1704	1720	rBV	1955196	2901166	65.64%	14.970%
7	14.392	1933	1939	1951	rVB	421235	652095	14.75%	3.365%
8	15.898	2187	2195	2215	rBV	1497589	2355106	53.29%	12.152%
9	17.157	2403	2409	2425	rBV	480311	794782	17.98%	4.101%
10	19.733	2841	2847	2856	rBV	3614327	4419609	100.00%	22.805%
11	21.269	3103	3108	3115	rBV	551140	780625	17.66%	4.028%
12	23.645	3506	3512	3521	rVB2	285609	638832	14.45%	3.296%




Sum of corrected areas: 19379657

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008447.D
Acq On : 16 Dec 2021 11:45
Operator : CG/JU
Sample : PB141458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141458BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

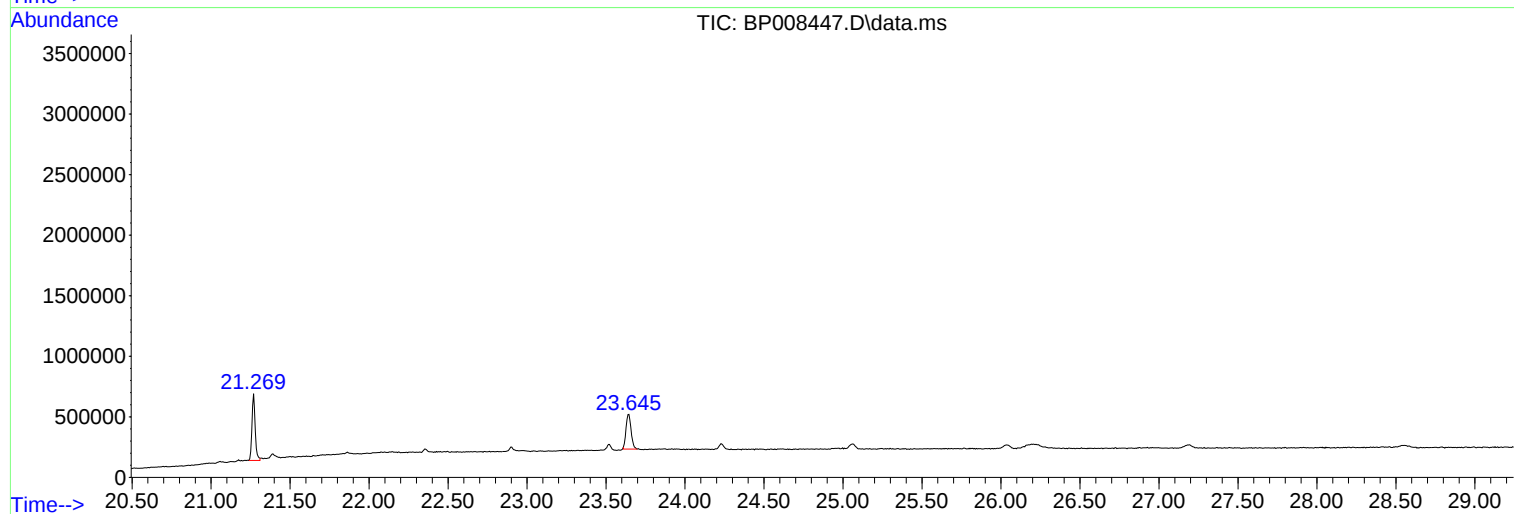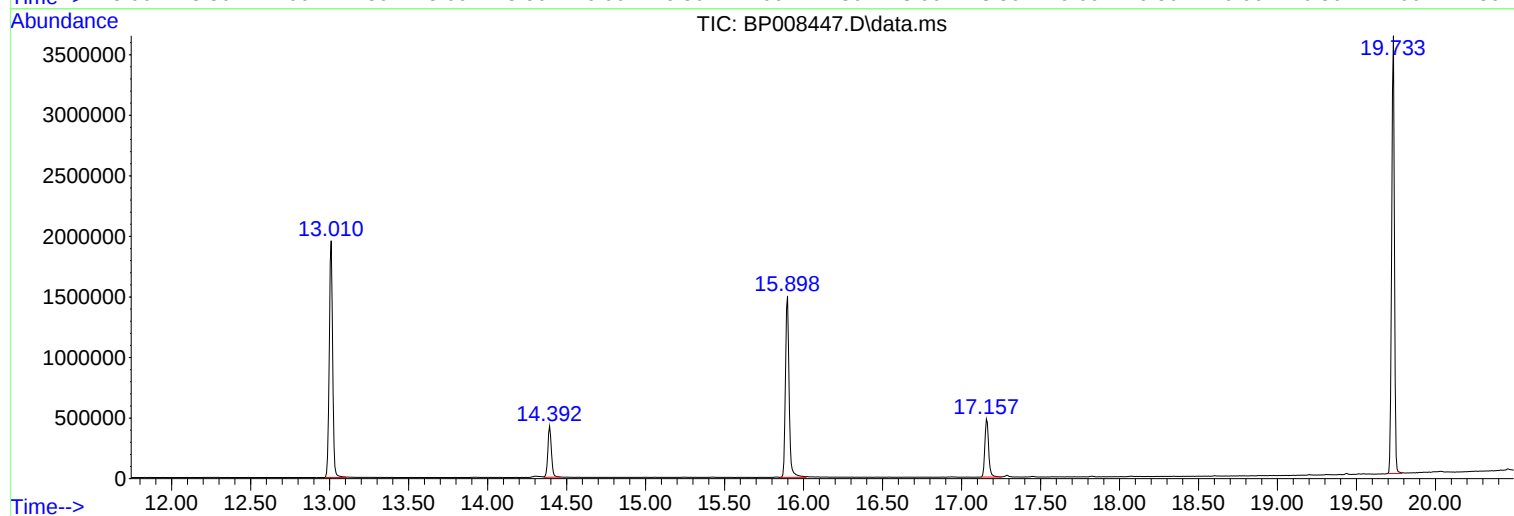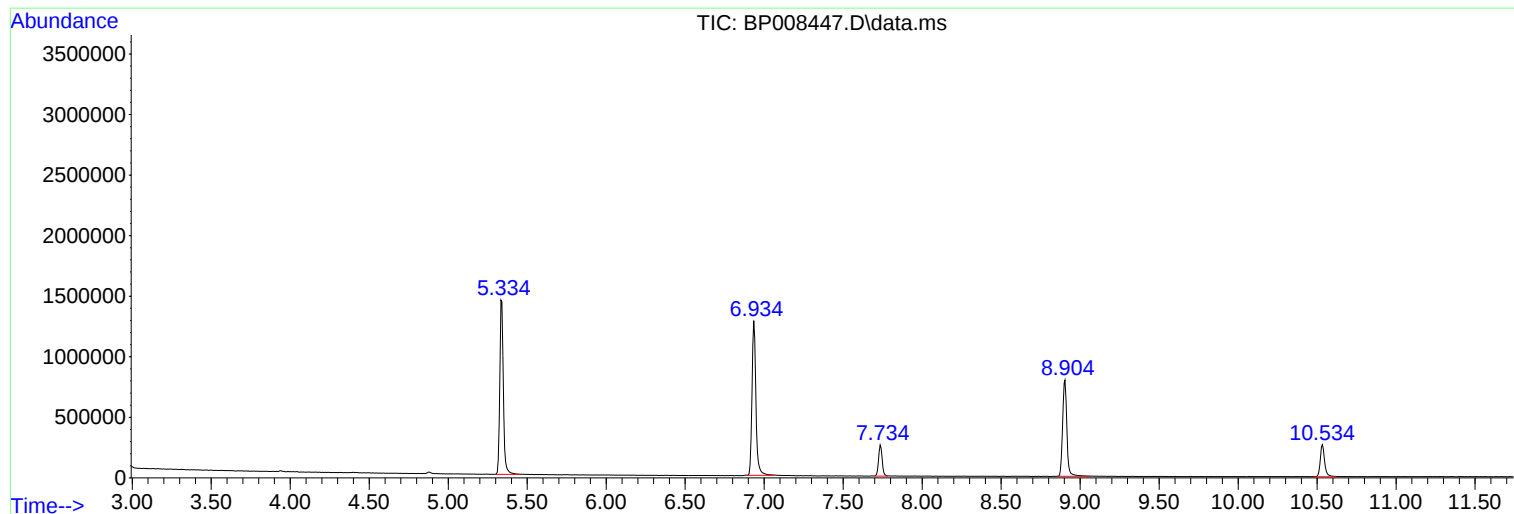

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008447.D
Acq On : 16 Dec 2021 11:45
Operator : CG/JU
Sample : PB141458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141458BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008447.D
Acq On : 16 Dec 2021 11:45
Operator : CG/JU
Sample : PB141458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141458BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------