
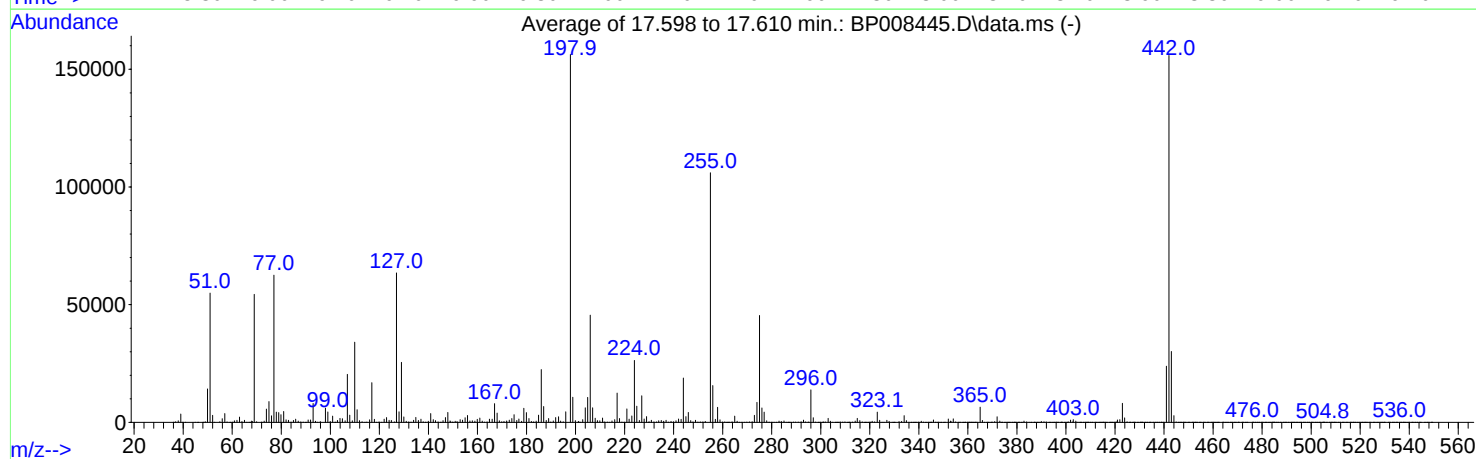


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
 Data File : BP008445.D
 Acq On : 16 Dec 2021 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 17:59:47 2021

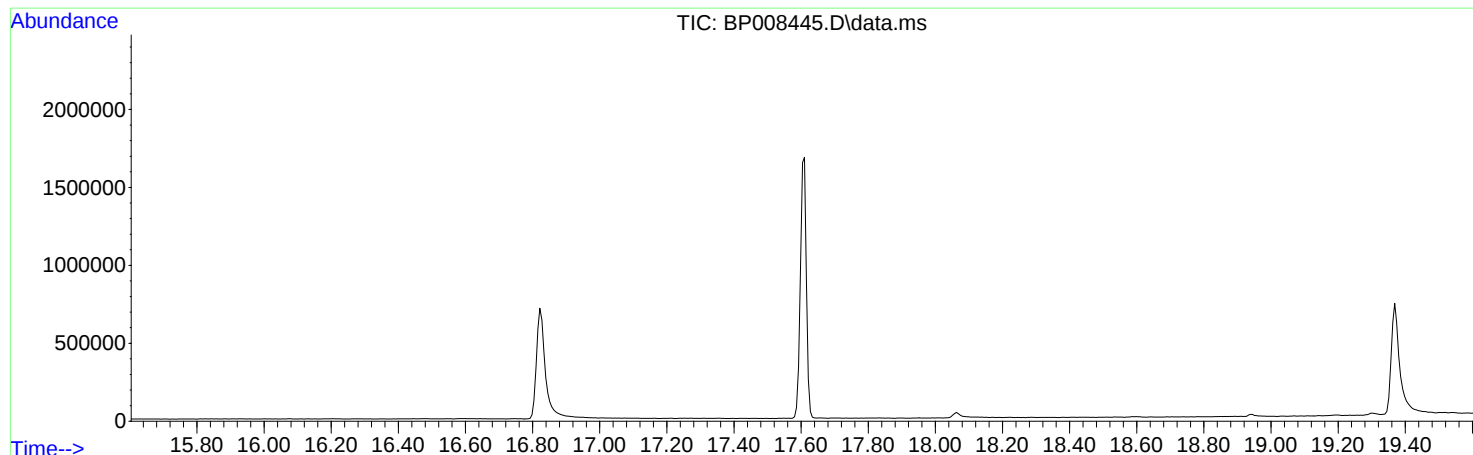




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	54941	PASS
68	69	0.00	2	0.9	515	PASS
69	198	0.00	100	34.8	54387	PASS
70	69	0.00	2	0.6	301	PASS
127	198	10	80	40.6	63520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156286	PASS
199	198	5	9	6.8	10660	PASS
275	198	10	60	29.1	45432	PASS
365	198	1	100	4.2	6490	PASS
441	198	0.01	100	15.3	23856	PASS
442	442	100	100	100.0	155877	PASS
443	442	15	24	19.3	30094	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
Data File : BP008445.D
Acq On : 16 Dec 2021 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 16 14:21:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 17:59:47 2021
Response via : Initial Calibration

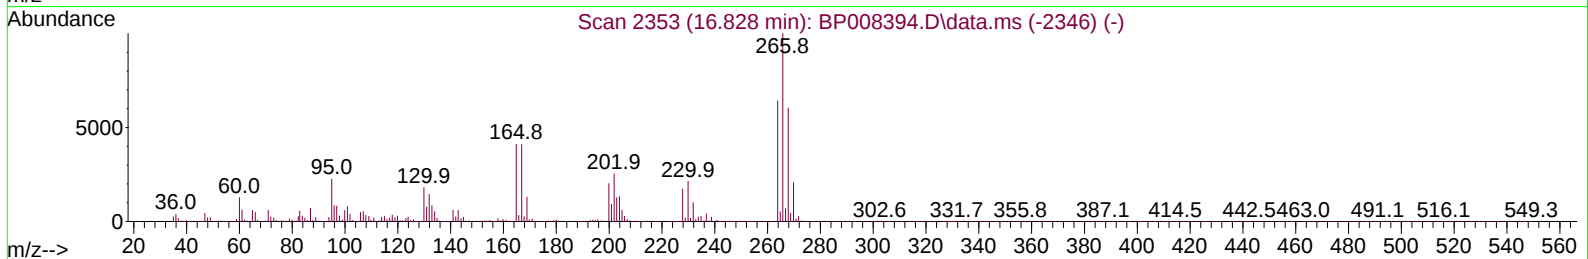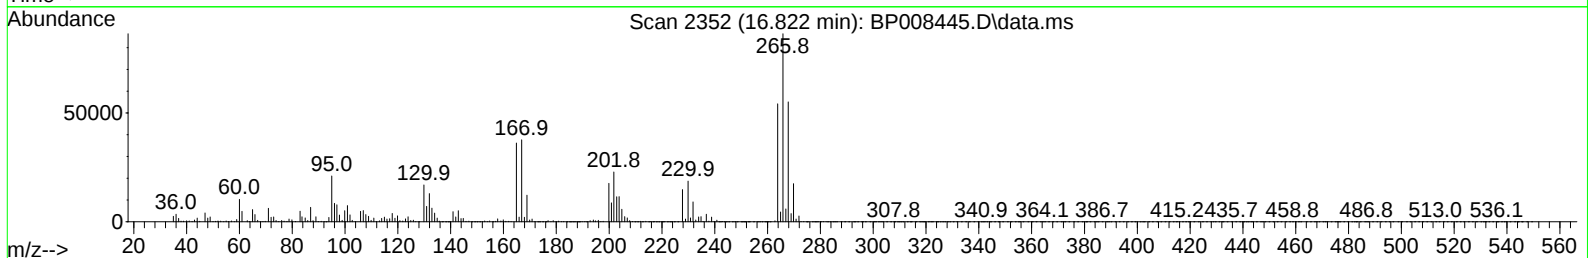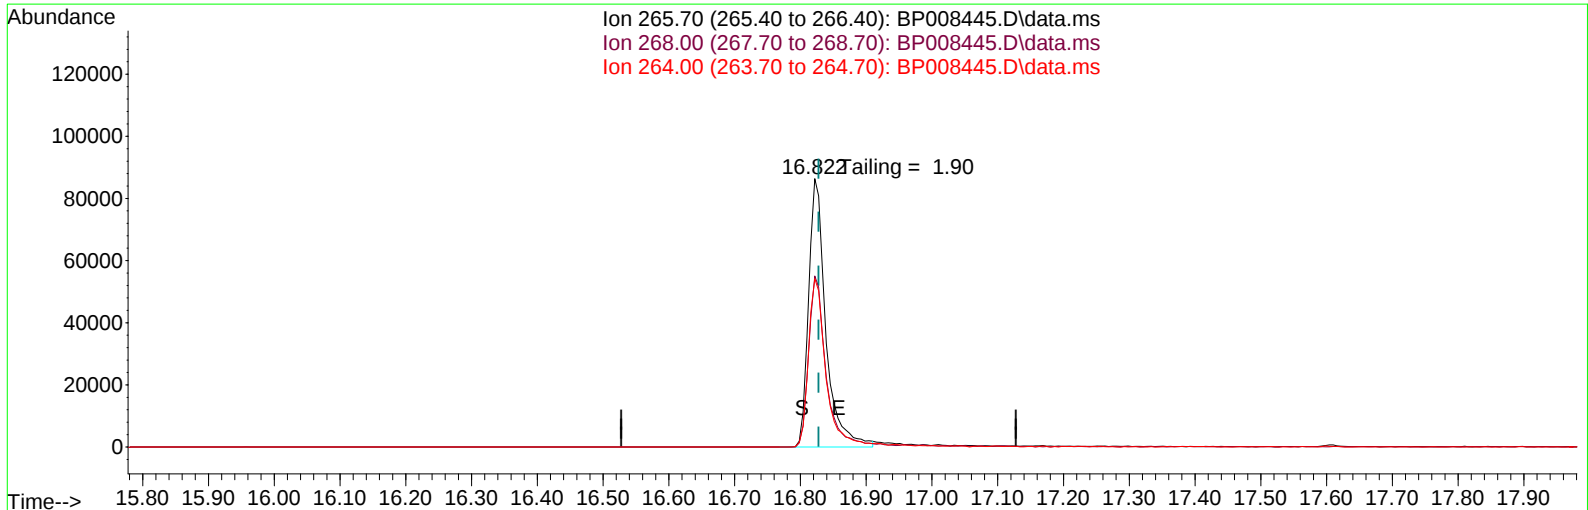

TIC: BP008445.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 733238.07 ng




response 159815

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.77
264.00	61.90	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121621\
 Data File : BP008445.D
 Acq On : 16 Dec 2021 10:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 14:21:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

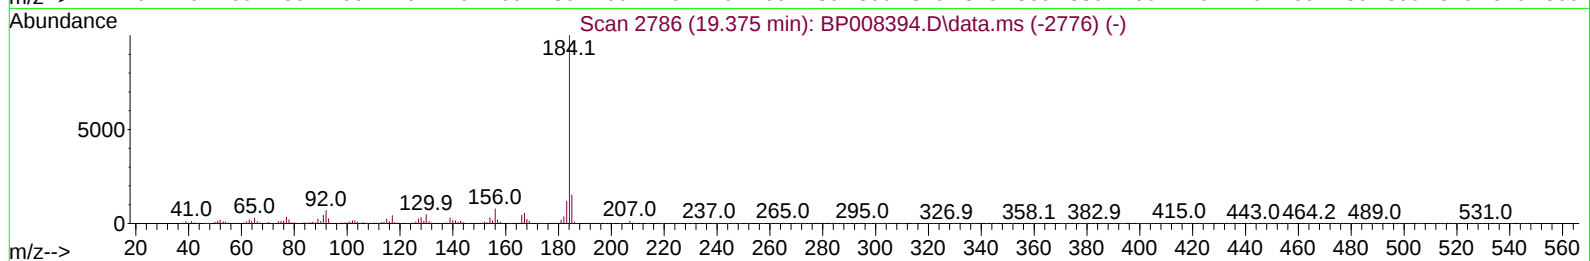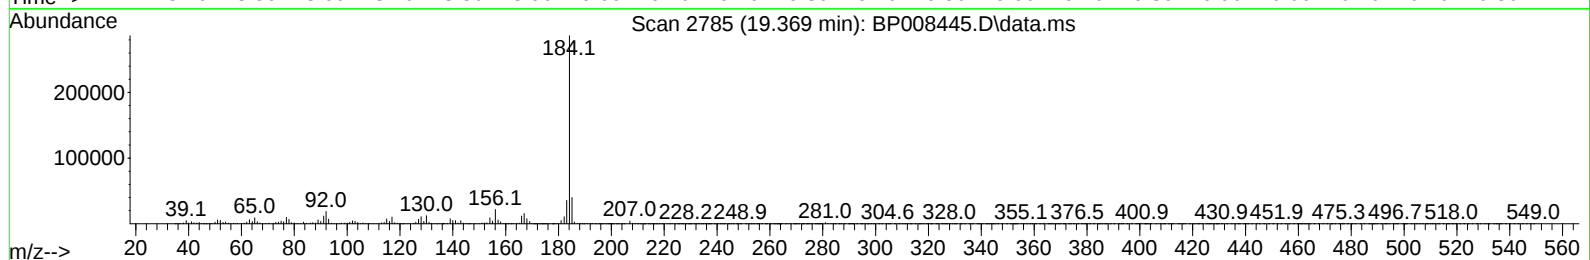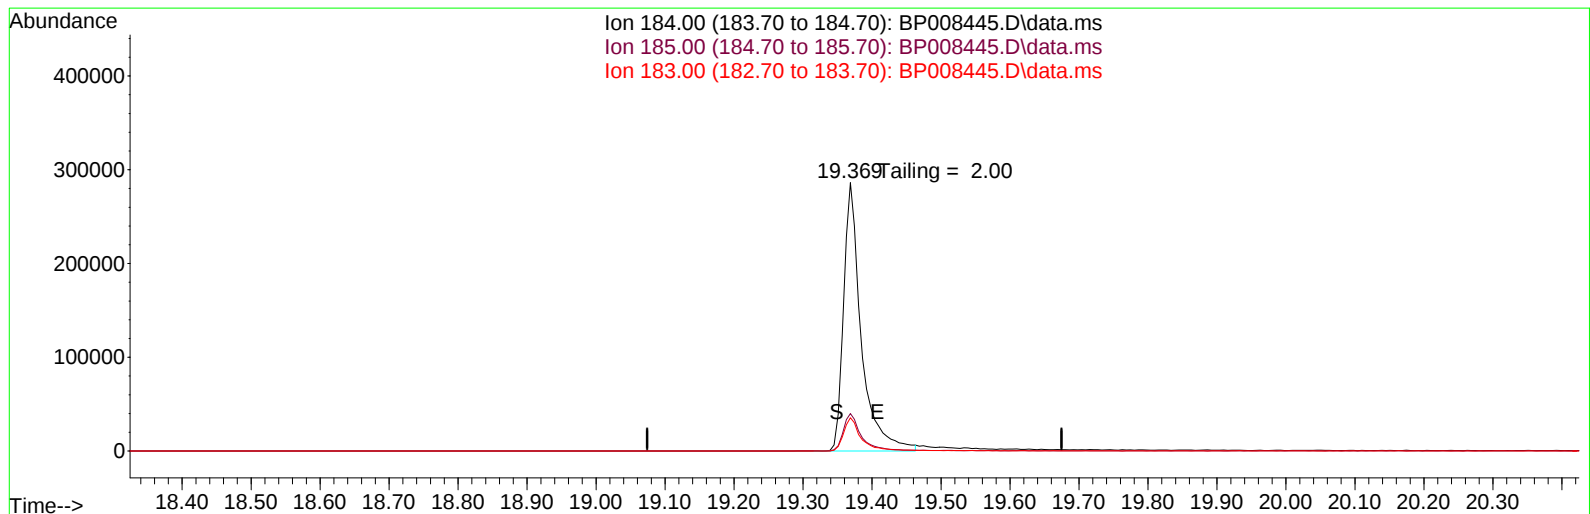

TIC: BP008445.D\data.ms

(77) Benzidine

19.369min (-0.006) 722466.90 ng m

response 512983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.99
183.00	11.40	12.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2021	BNA_P	BP008445.D
Compound Name	Response	Retention Time
DDT	845270	20.57
DDD	8881	20.14
DDE	1838	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10719	855989	1.25

Instrument :
BNA_P
ClientSampleId :
DFTPP