


Instrument :
BNA_P
ClientSampleId :

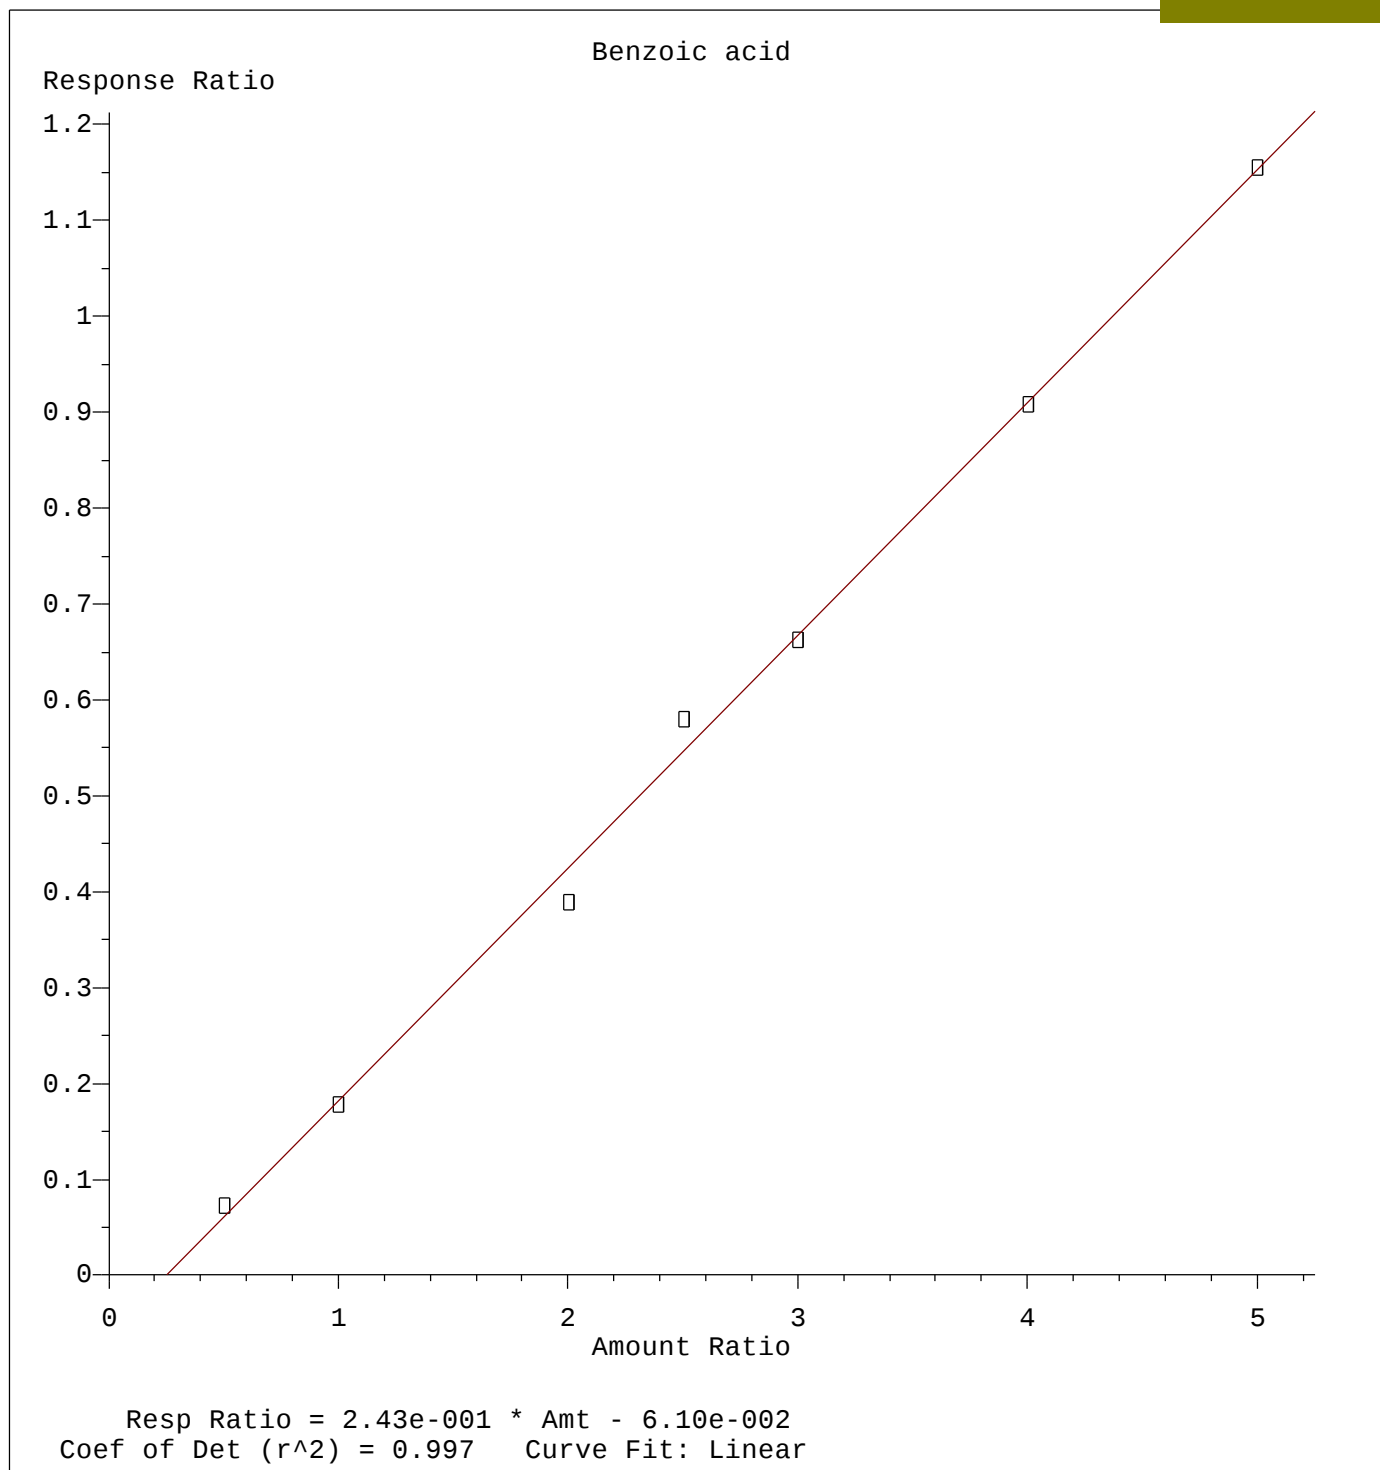

Method Name: Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
Calibration Table Last Updated: Fri Dec 20 03:20:39 2019