


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121919\
 Data File : BP001325.D
 Acq On : 19 Dec 2019 15:50
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP121919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 20 03:20:39 2019

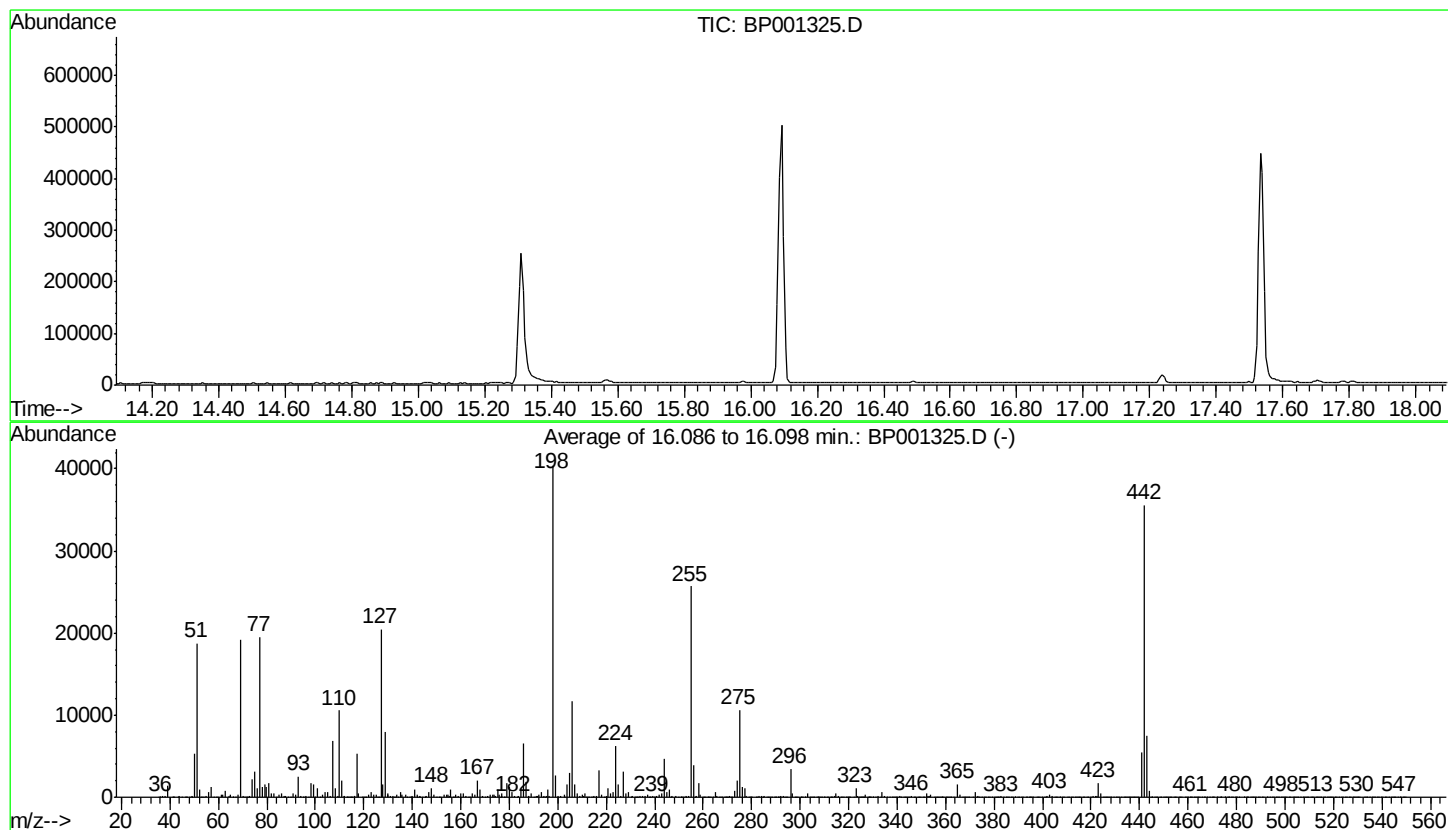

AutoFind: Scans 2380, 2381, 2382; Background Corrected with Scan 2373

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	18759	PASS
68	69	0.00	2	1.9	368	PASS
69	198	0.00	100	47.5	19165	PASS
70	69	0.00	2	0.5	97	PASS
127	198	10	80	50.6	20443	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40373	PASS
199	198	5	9	6.7	2705	PASS
275	198	10	60	26.4	10669	PASS
365	198	1	100	4.0	1627	PASS
441	198	0.01	100	13.7	5523	PASS
442	198	50	100	88.0	35544	PASS
443	442	15	24	20.9	7441	PASS