

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013125.D
 Acq On : 19 Dec 2022 14:16
 Operator : CG/JU
 Sample : N5925-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXU8

Quant Time: Dec 19 21:46:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	660295	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	2743392	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.604	164	1736226	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188	3686052	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	2376327	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	2168196	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	55977	3.625	ng/uL	0.00
4) Pyridine-d5	3.775	84	159641	3.639	ng/ul	0.01
7) Phenol-d5	7.116	99	955080	17.758	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	717914	22.128	ng/ul	0.00
11) 2-Chlorophenol-d4	7.487	132	832027	19.652	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	636844	14.451	ng/ul	0.00
21) Nitrobenzene-d5	9.128	128	415486	20.613	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	469420	20.686	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.393	165	865353	19.633	ng/ul	0.00
31) 4-Chloroaniline-d4	10.916	131	846179	13.599	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	2966832	22.234	ng/ul	0.00
49) Acenaphthylene-d8	14.298	160	3009993	20.529	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	303504	12.645	ng/ul	0.00
60) Fluorene-d10	15.598	176	2451634	21.717	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	352290	14.852	ng/ul	0.00
73) Anthracene-d10	17.463	188	3431373	20.634	ng/ul	0.00
81) Pyrene-d10	19.692	212	3585397	26.286	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.769	264	2073558	19.187	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.099	77	314119	14.916	ng/ul	97
10) Bis(2-Chloroethyl)ether	7.393	93	1026146	22.991	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013125.D
Acq On : 19 Dec 2022 14:16
Operator : CG/JU
Sample : N5925-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXU8

Quant Time: Dec 19 21:46:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration




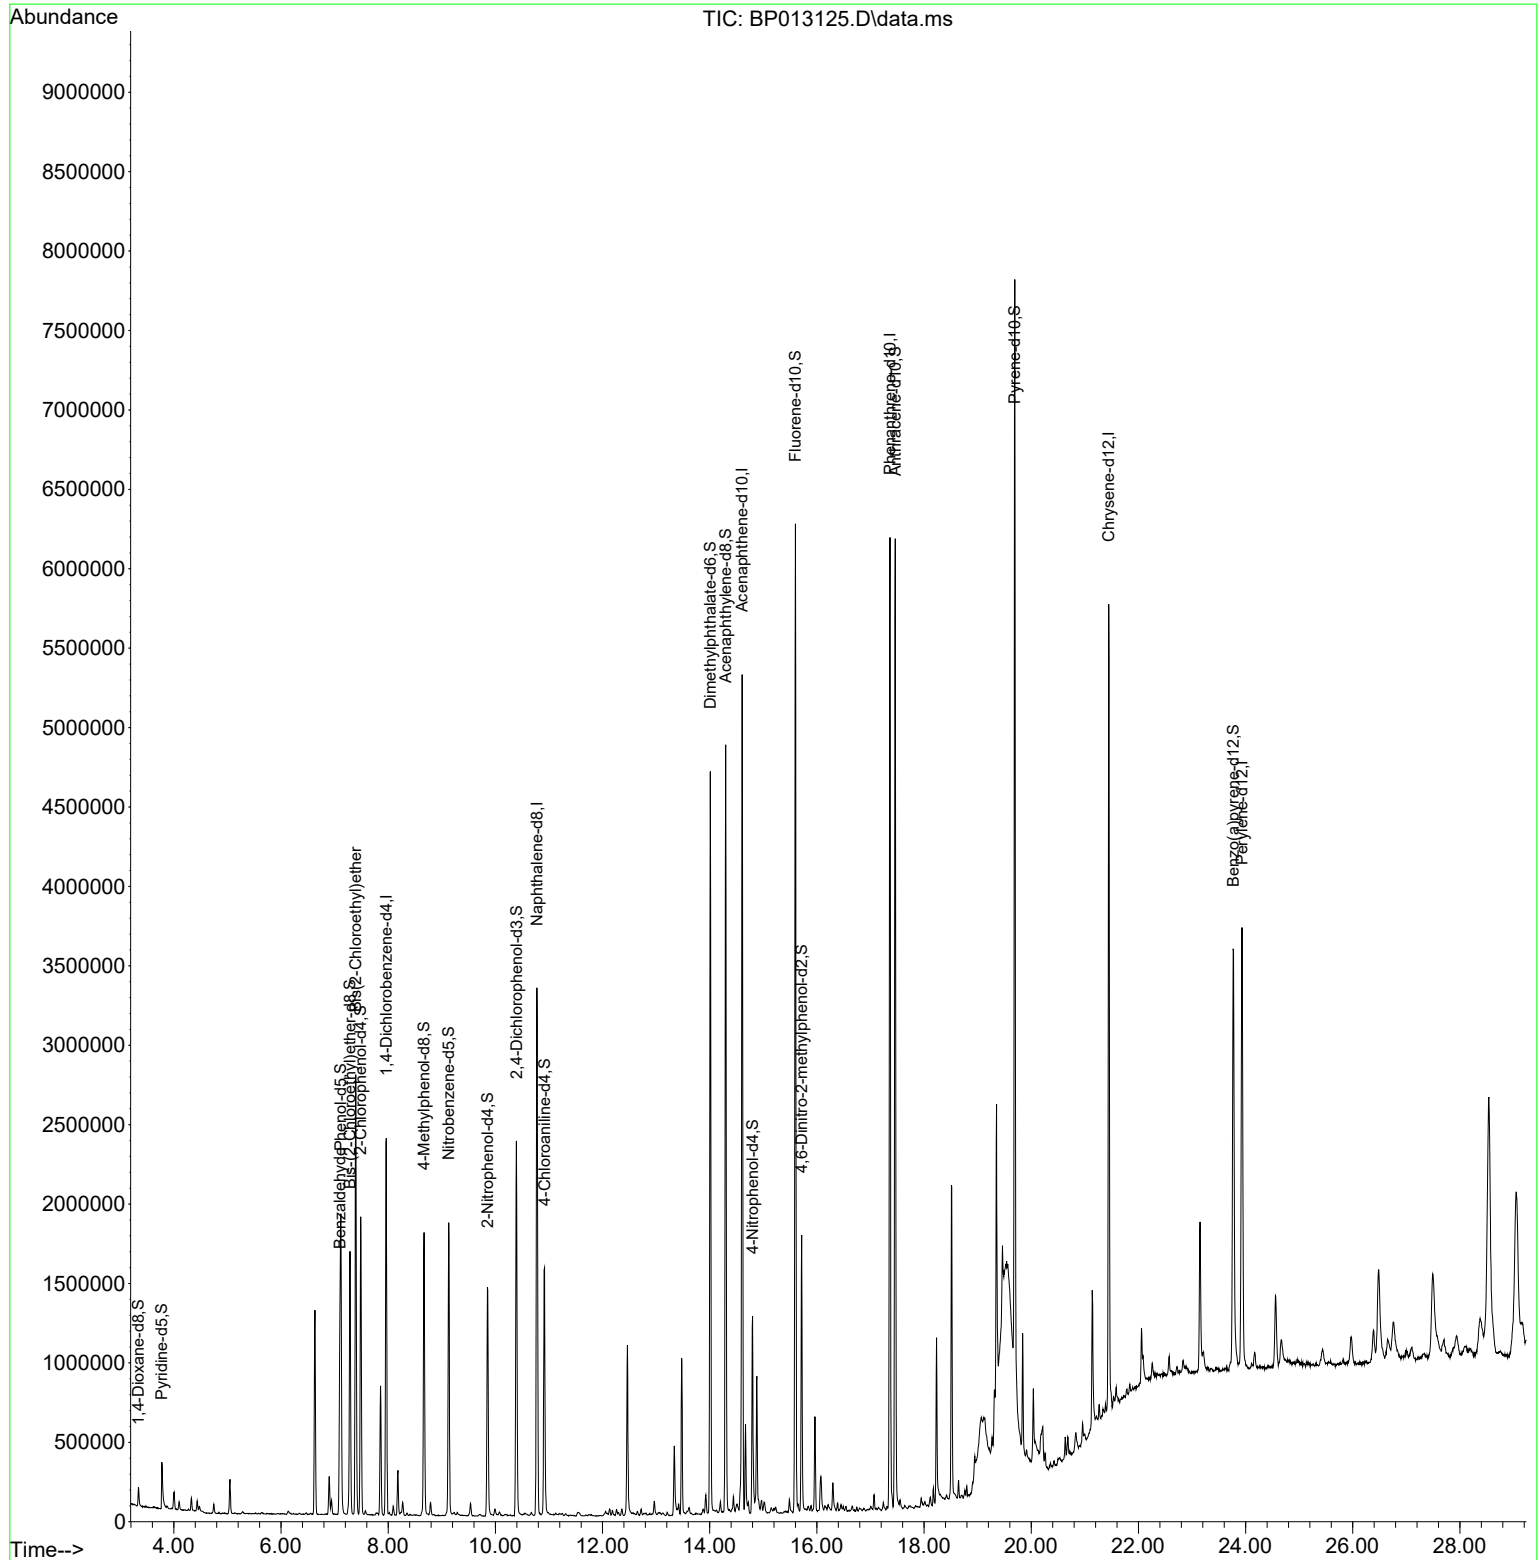


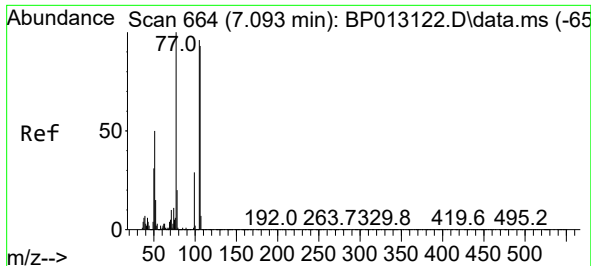

#6
Benzaldehyde
Concen: 14.916 ng/ul
RT: 7.099 min Scan# 60
Delta R.T. 0.006 min
Lab File: BP013125.D
Acq: 19 Dec 2022 14:16

Instrument :
BNA_P
ClientSampleId :
DBXU8

Tgt Ion: 77 Resp: 314119
Ion Ratio Lower Upper
77 100
105 98.2 81.5 122.3
106 94.5 76.9 115.3

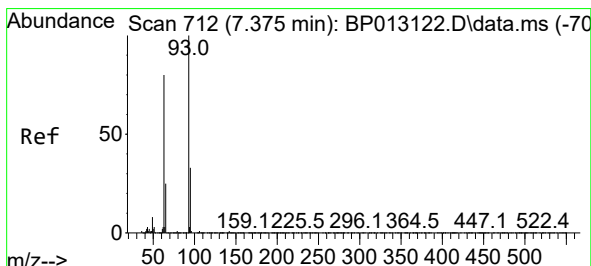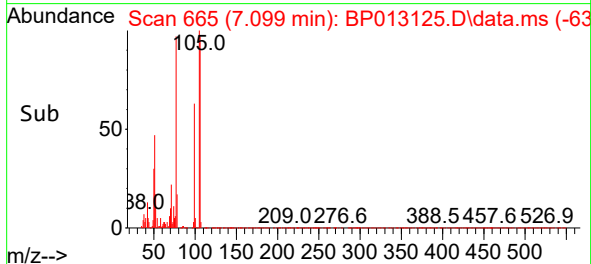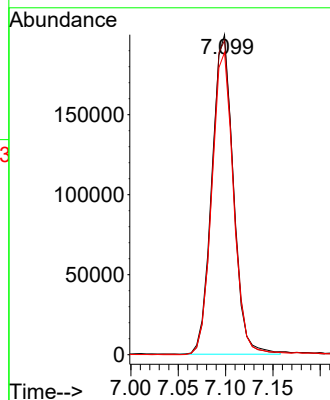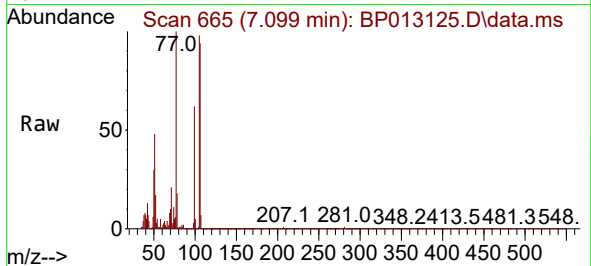

#10
Bis(2-Chloroethyl)ether
Concen: 22.991 ng/ul
RT: 7.393 min Scan# 715
Delta R.T. 0.018 min
Lab File: BP013125.D
Acq: 19 Dec 2022 14:16

Tgt Ion: 93 Resp: 1026146
Ion Ratio Lower Upper
93 100
63 2.1 59.8 89.8#
95 2.1 26.4 39.6#

