

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013136.D
 Acq On : 19 Dec 2022 20:38
 Operator : CG/JU
 Sample : N6006-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYA0

Quant Time: Dec 19 21:48:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	559202	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	2405295	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	1564772	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	3391799	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2301189	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	2221551	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	67395	5.153	ng/uL	0.00
4) Pyridine-d5	3.775	84	184713	4.972	ng/ul	0.01
7) Phenol-d5	7.111	99	1242688	27.283	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	893991	32.537	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	1076967	30.036	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	868875	23.281	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	571900	32.361	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	623580	31.342	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1121224	29.014	ng/ul	0.00
31) 4-Chloroaniline-d4	10.905	131	846239	15.511	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	3721291	30.944	ng/ul	0.00
49) Acenaphthylene-d8	14.293	160	4191348	31.718	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	375325	17.350	ng/ul	0.00
60) Fluorene-d10	15.592	176	3293212	32.369	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	497158	22.777	ng/ul	0.00
73) Anthracene-d10	17.451	188	4724890	30.878	ng/ul	0.00
81) Pyrene-d10	19.686	212	5244064	39.701	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	3321167	29.993	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.093	77	28134	1.577	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013136.D
Acq On : 19 Dec 2022 20:38
Operator : CG/JU
Sample : N6006-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYA0

Quant Time: Dec 19 21:48:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

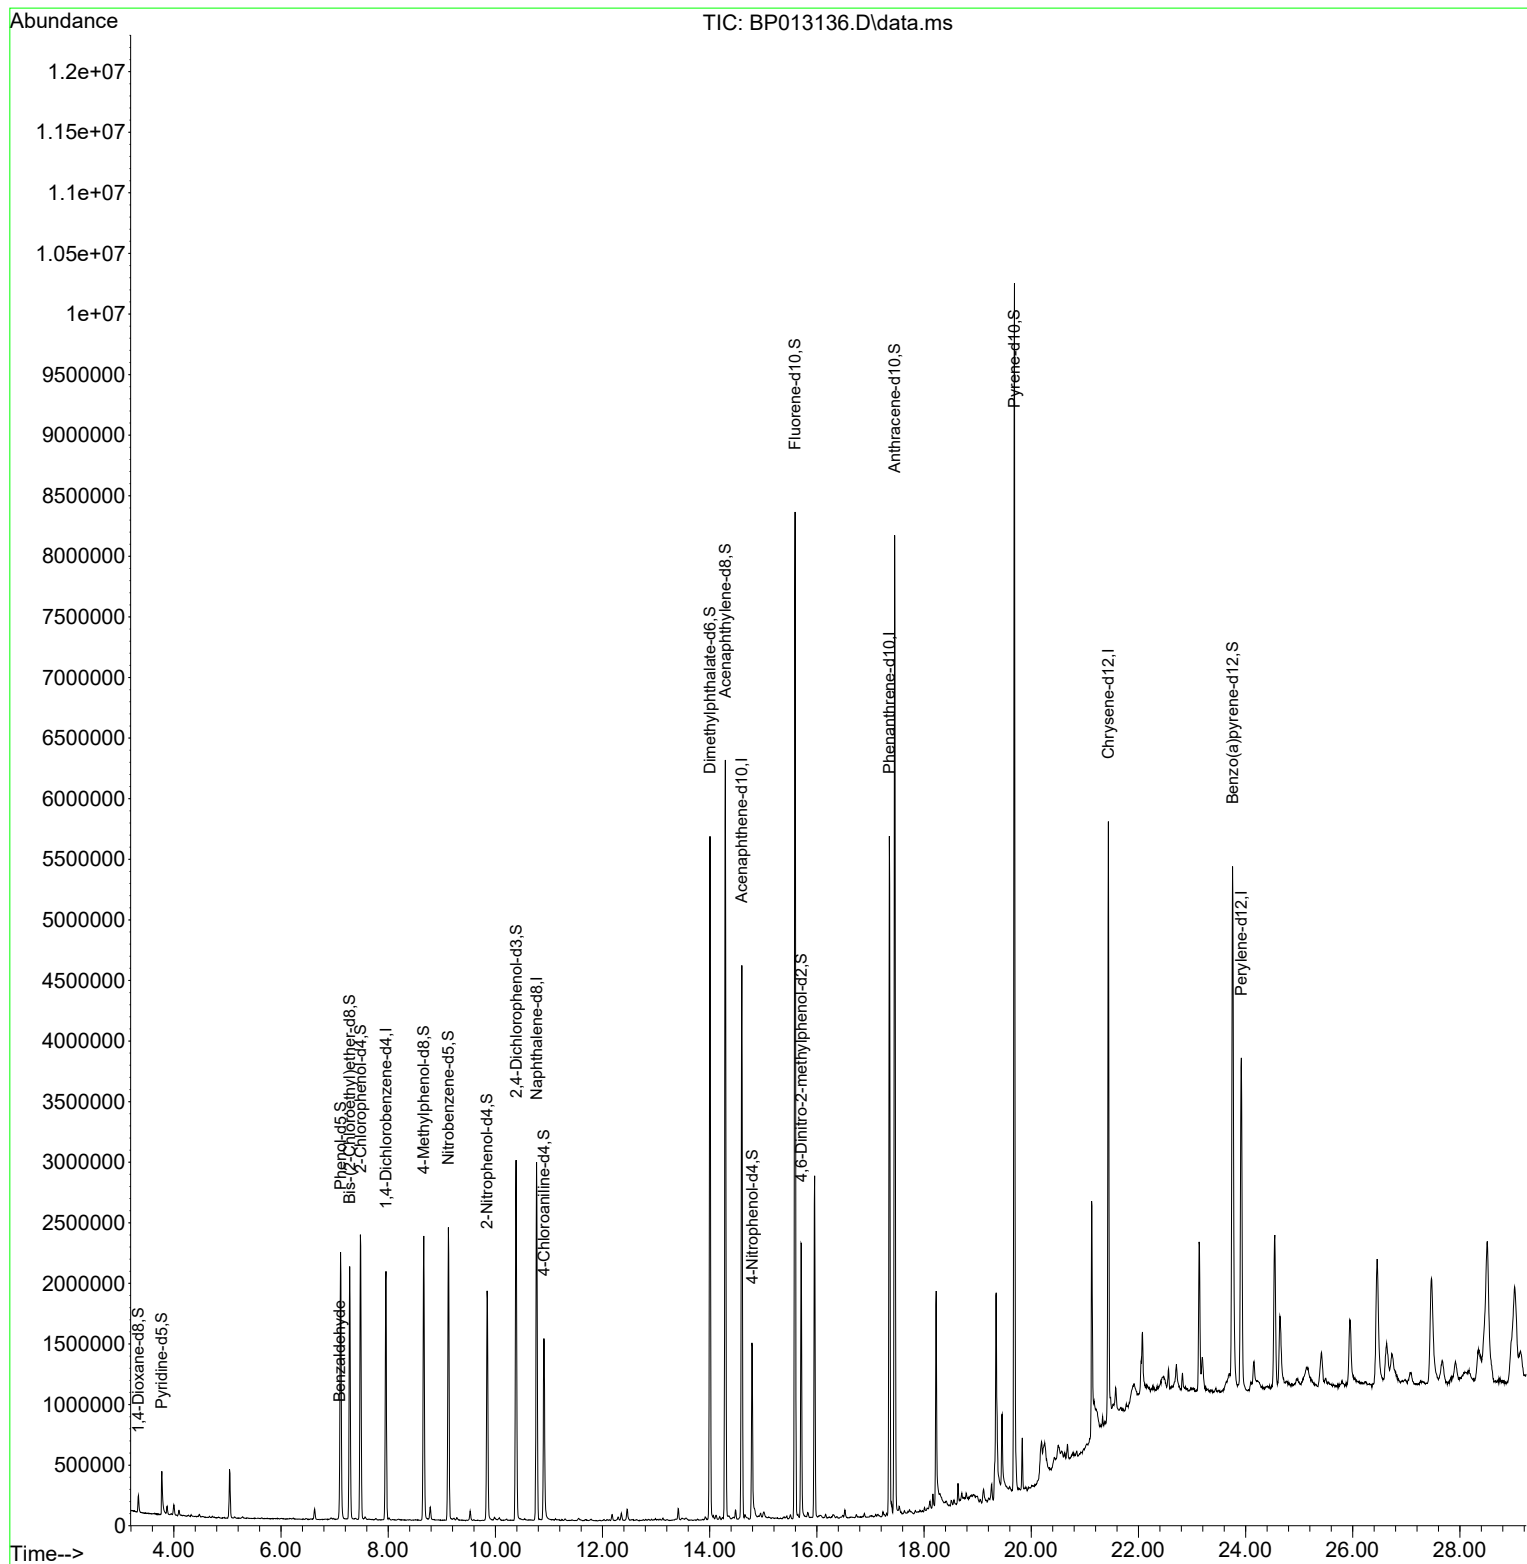

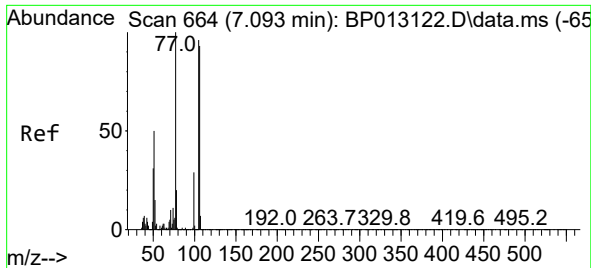

#6
Benzaldehyde
Concen: 1.577 ng/ul
RT: 7.093 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP013136.D
Acq: 19 Dec 2022 20:38

Instrument :
BNA_P
ClientSampleId :
DBYA0

Tgt Ion:	77	Resp:	28134
Ion	Ratio	Lower	Upper
77	100		
105	96.6	81.5	122.3
106	92.8	76.9	115.3

