

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013154.D
 Acq On : 20 Dec 2022 07:58
 Operator : CG/JU
 Sample : N6003-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXX2

Quant Time: Dec 20 21:43:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	494062	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	1942141	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	1107456	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	2182803	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2165749	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	2674305	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	74298	6.430	ng/uL	0.00
4) Pyridine-d5	3.764	84	550746	16.778	ng/ul	0.00
7) Phenol-d5	7.111	99	1327643	32.991	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	853934	35.176	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	1099441	34.705	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	871830	26.440	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	534656	37.469	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	603609	37.574	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1051715	33.705	ng/ul	0.00
31) 4-Chloroaniline-d4	10.905	131	1064282	24.160	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	2886175	33.910	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	3404453	36.402	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	402120	26.265	ng/ul	0.00
60) Fluorene-d10	15.587	176	2498451	34.698	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	385403	27.437	ng/ul	0.00
73) Anthracene-d10	17.451	188	3453041	35.065	ng/ul	0.00
81) Pyrene-d10	19.681	212	4321141	34.760	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	4921859	36.924	ng/ul	0.00


Target Compounds					Qvalue
16) Acetophenone	8.787	105	50981	1.008 ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013154.D
Acq On : 20 Dec 2022 07:58
Operator : CG/JU
Sample : N6003-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXX2

Quant Time: Dec 20 21:43:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

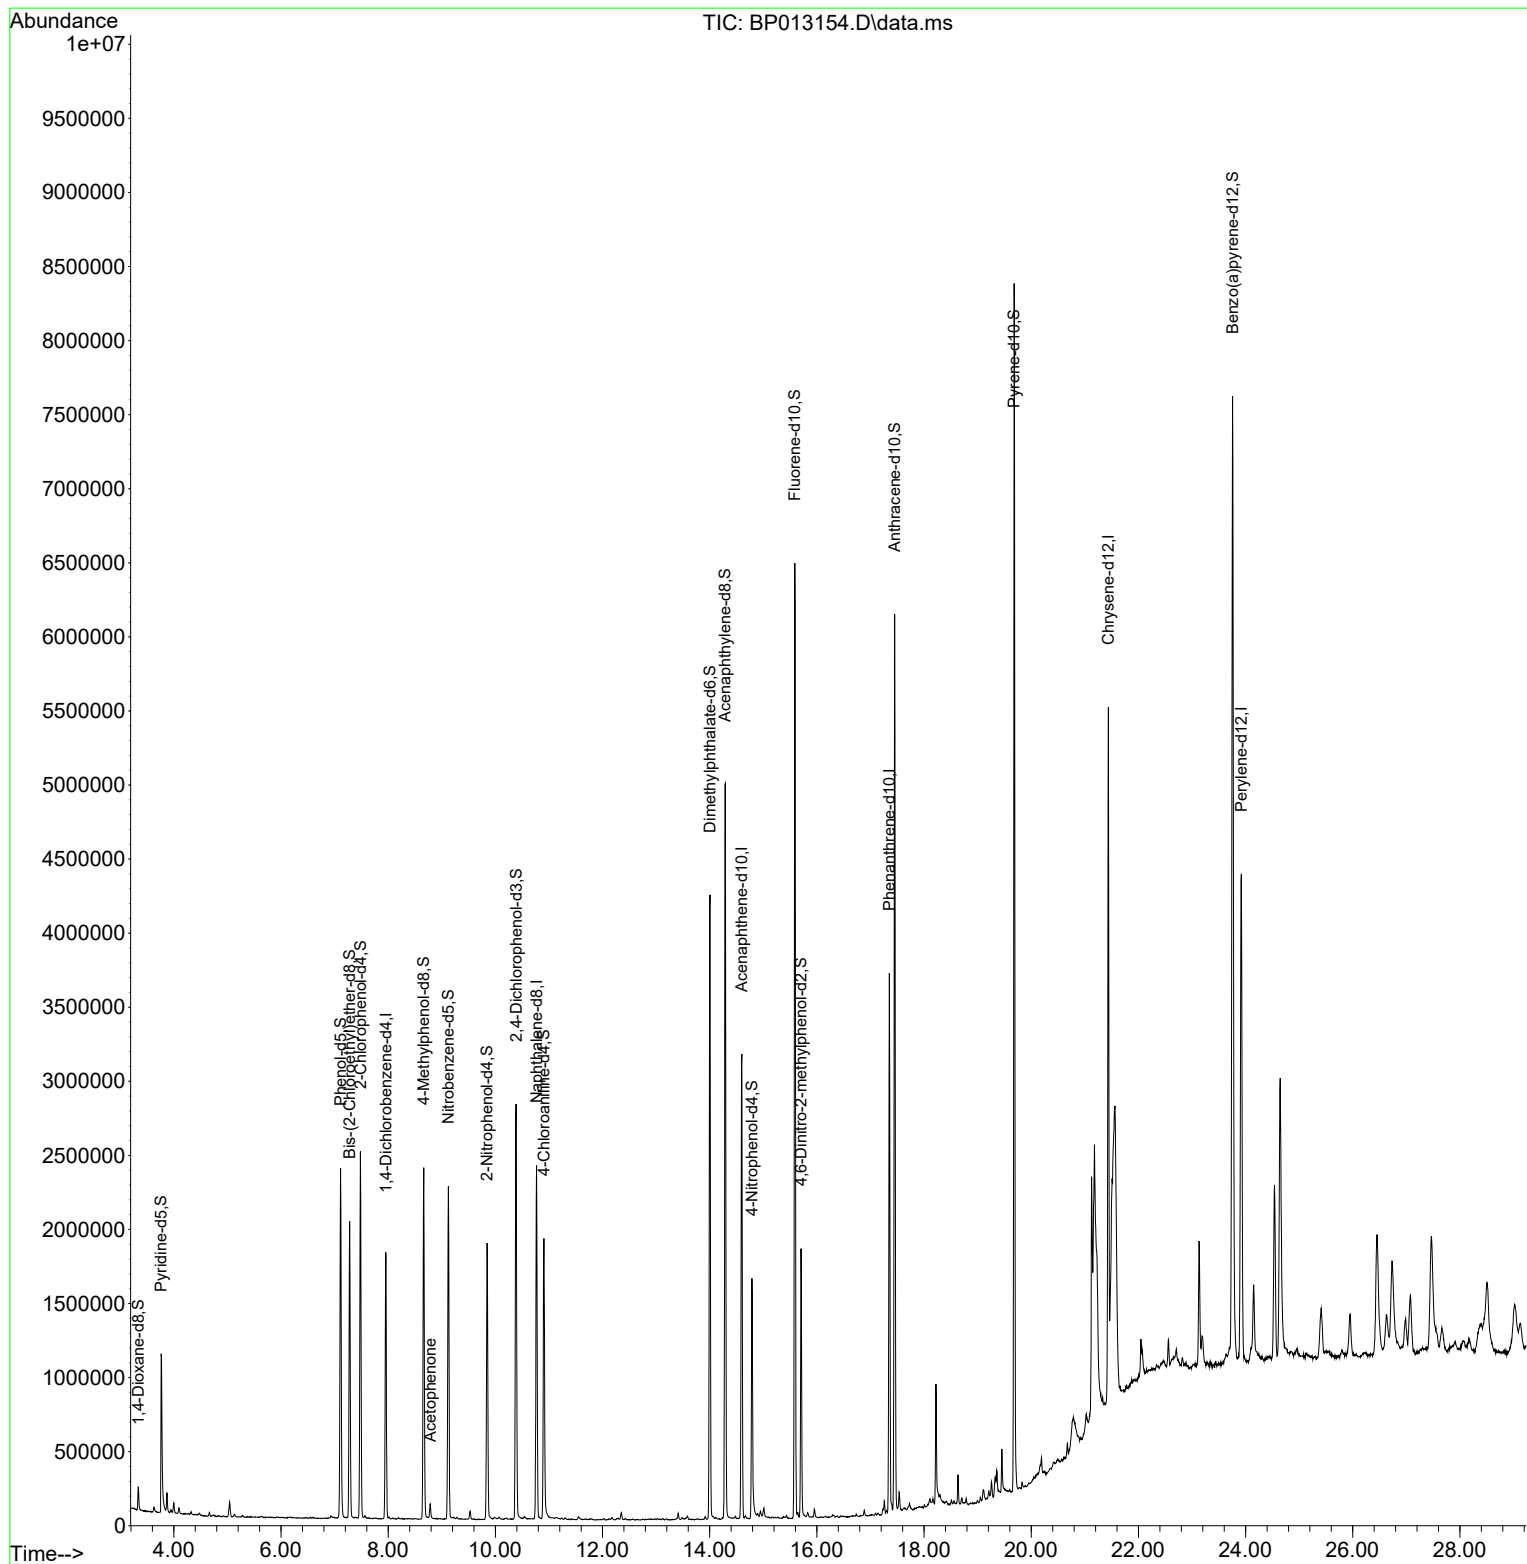

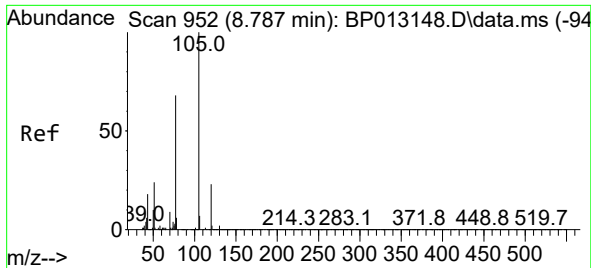

#16
 Acetophenone
 Concen: 1.008 ng/ul
 RT: 8.787 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP013154.D
 Acq: 20 Dec 2022 07:58

Instrument :
 BNA_P
 ClientSampleId :
 DBXX2

Tgt Ion:	105	Resp:	50981
Ion	Ratio	Lower	Upper
105	100		
77	76.4	59.3	88.9
51	29.9	19.6	29.4#

