

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013157.D
 Acq On : 20 Dec 2022 09:40
 Operator : CG/JU
 Sample : N6003-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXX3

Quant Time: Dec 20 21:44:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	415703	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	1620873	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.593	164	925597	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	1833742	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	1850974	20.000	ng/ul	0.00
88) Perylene-d12	23.916	264	2276280	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	56871	5.849	ng/uL	0.00
4) Pyridine-d5	3.770	84	275020	9.958	ng/ul	0.00
7) Phenol-d5	7.111	99	1009049	29.801	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	657226	32.176	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	839648	31.501	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	628939	22.669	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	402603	33.807	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	455045	33.940	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	801459	30.776	ng/ul	0.00
31) 4-Chloroaniline-d4	10.904	131	889152	24.185	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	2275180	31.983	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	2629507	33.640	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	286824	22.415	ng/ul	0.00
60) Fluorene-d10	15.587	176	1966686	32.679	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	272546	23.096	ng/ul	0.00
73) Anthracene-d10	17.451	188	2721336	32.895	ng/ul	0.00
81) Pyrene-d10	19.680	212	3445761	32.432	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	3892916	34.311	ng/ul	0.00
Target Compounds						
6) Benzaldehyde	7.093	77	36296	2.738	ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.333	149	74377	1.097	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013157.D
Acq On : 20 Dec 2022 09:40
Operator : CG/JU
Sample : N6003-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXX3

Quant Time: Dec 20 21:44:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration




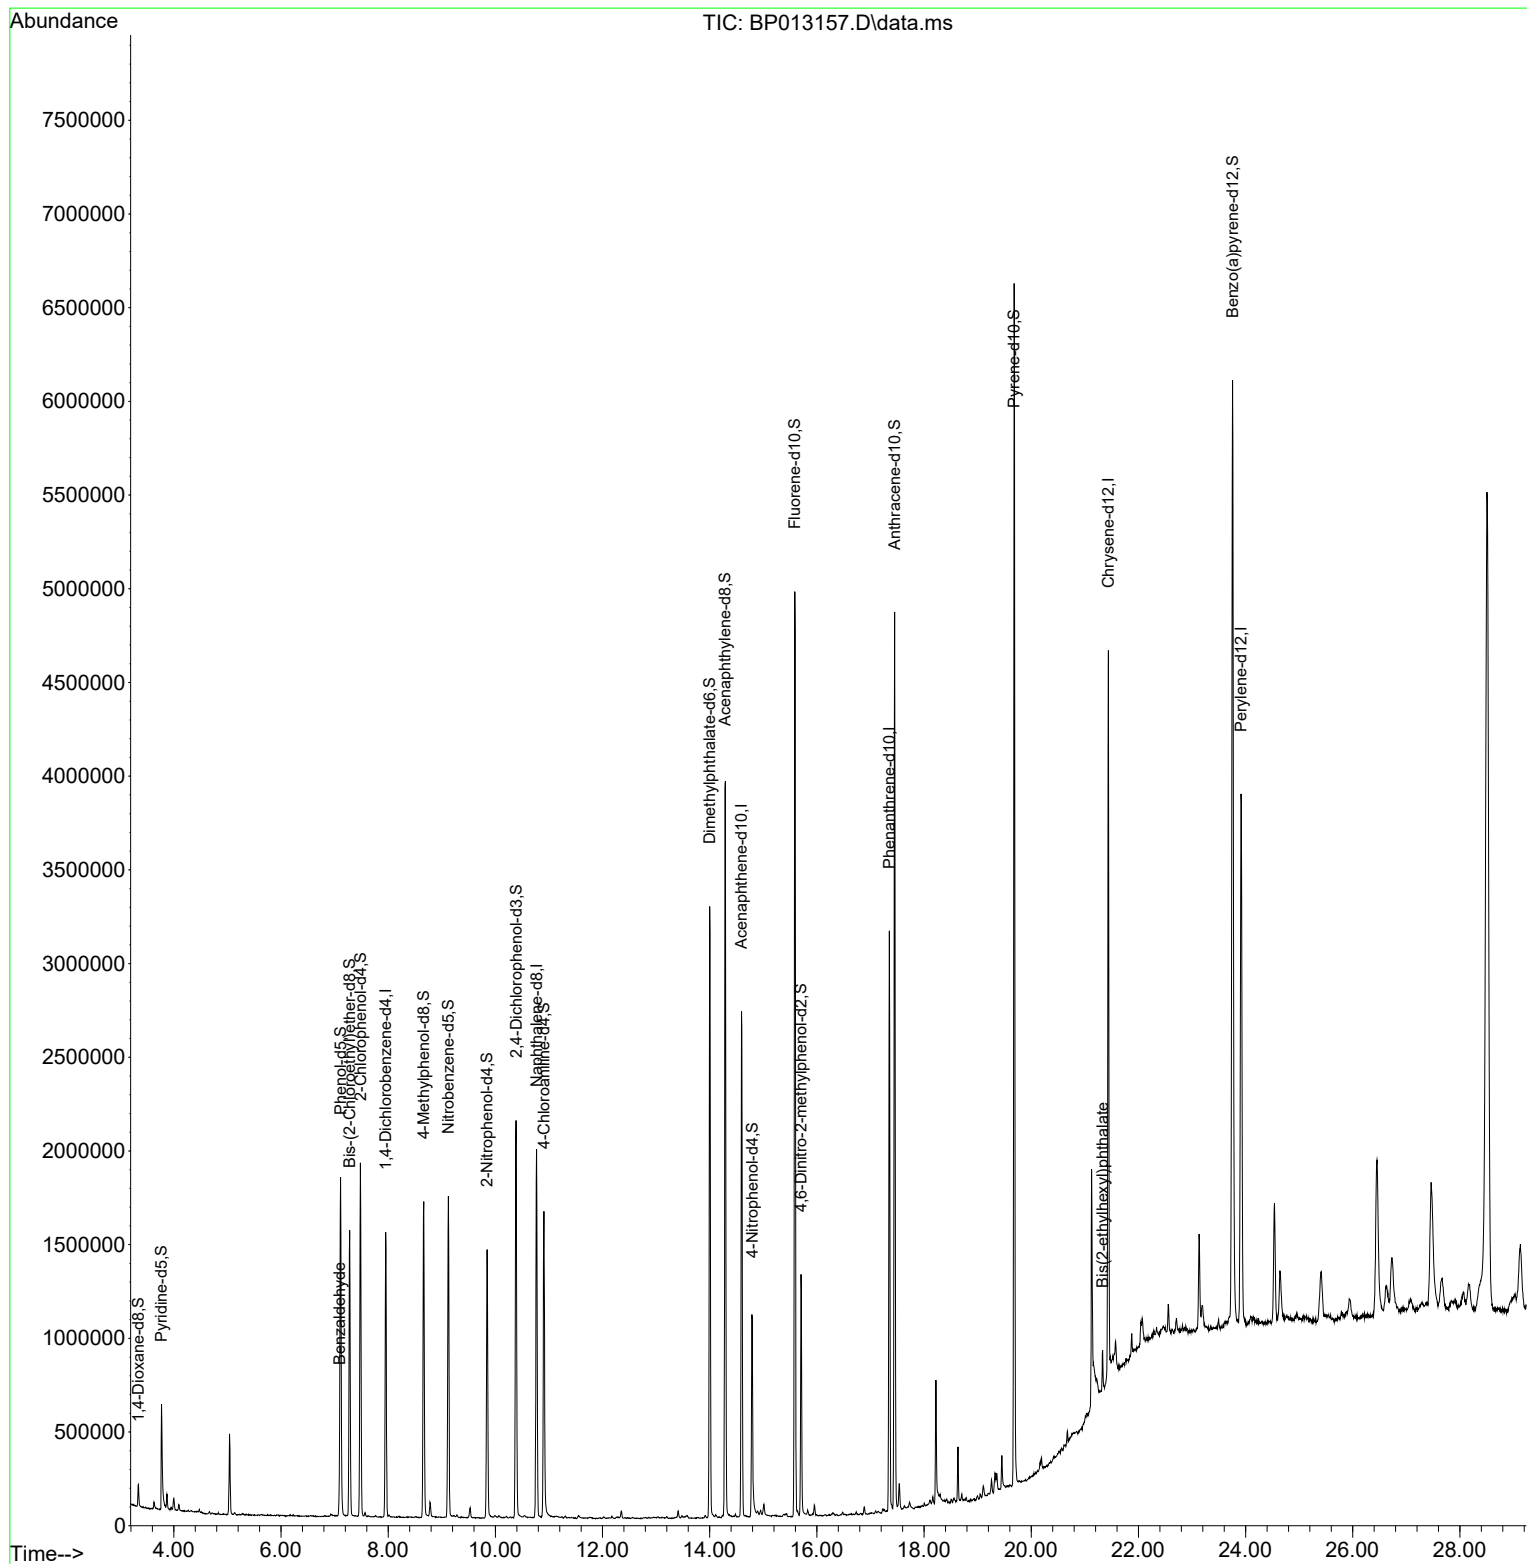


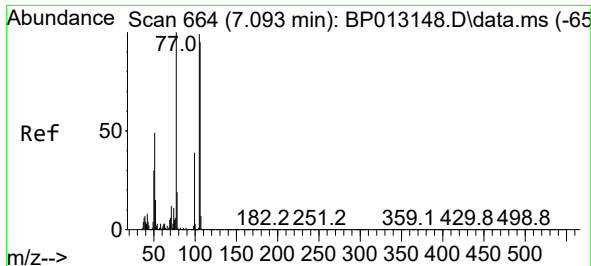

#6
Benzaldehyde
Concen: 2.738 ng/ul
RT: 7.093 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP013157.D
Acq: 20 Dec 2022 09:40

Instrument :
BNA_P
ClientSampleId :
DBXX3

Tgt Ion: 77 Resp: 36296
Ion Ratio Lower Upper
77 100
105 96.6 81.5 122.3
106 89.8 76.9 115.3

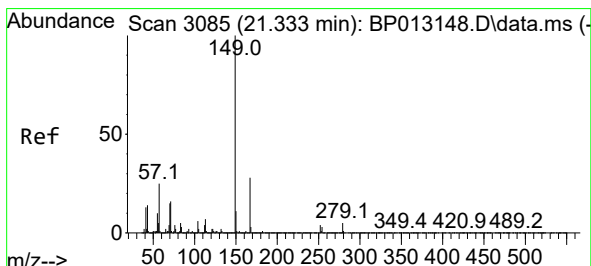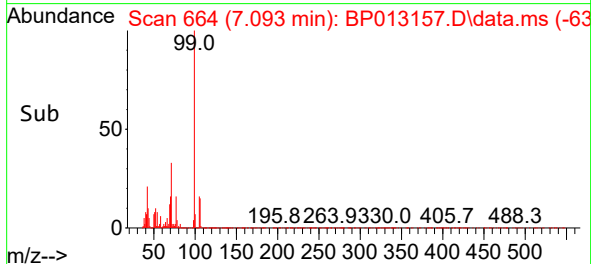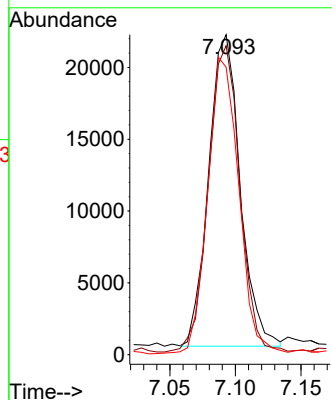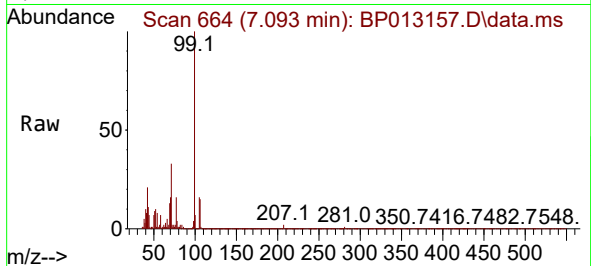

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.097 ng/ul
RT: 21.333 min Scan# 3085
Delta R.T. 0.000 min
Lab File: BP013157.D
Acq: 20 Dec 2022 09:40

Tgt Ion: 149 Resp: 74377
Ion Ratio Lower Upper
149 100
167 26.8 22.5 33.7
279 5.1 3.8 5.8

