

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013165.D
 Acq On : 20 Dec 2022 14:12
 Operator : CG/JU
 Sample : N6003-15
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXQ8

Quant Time: Dec 20 21:46:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	529320	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	2080900	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	1254728	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	2731045	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2841141	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	3259818	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	62159	5.021	ng/uL	0.00
4) Pyridine-d5	3.770	84	341018	9.697	ng/ul	0.00
7) Phenol-d5	7.111	99	1259595	29.215	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	780972	30.028	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	1047067	30.850	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	767222	21.718	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	499458	32.668	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	573177	33.300	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1036989	31.017	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	146999	3.115	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	3013949	31.255	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	3409822	32.180	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	457524	26.376	ng/ul	0.00
60) Fluorene-d10	15.587	176	2641429	32.378	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	279194	15.886	ng/ul	0.00
73) Anthracene-d10	17.451	188	4134962	33.560	ng/ul	0.00
81) Pyrene-d10	19.686	212	5394499	33.079	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.769	264	5592414	34.419	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.087	77	82465	4.885	ng/ul	90
10) Bis(2-Chloroethyl)ether	7.387	93	1267106	35.415	ng/ul#	24
86) Bis(2-ethylhexyl)phtha...	21.333	149	119663	1.150	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013165.D
Acq On : 20 Dec 2022 14:12
Operator : CG/JU
Sample : N6003-15
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXQ8

Quant Time: Dec 20 21:46:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration




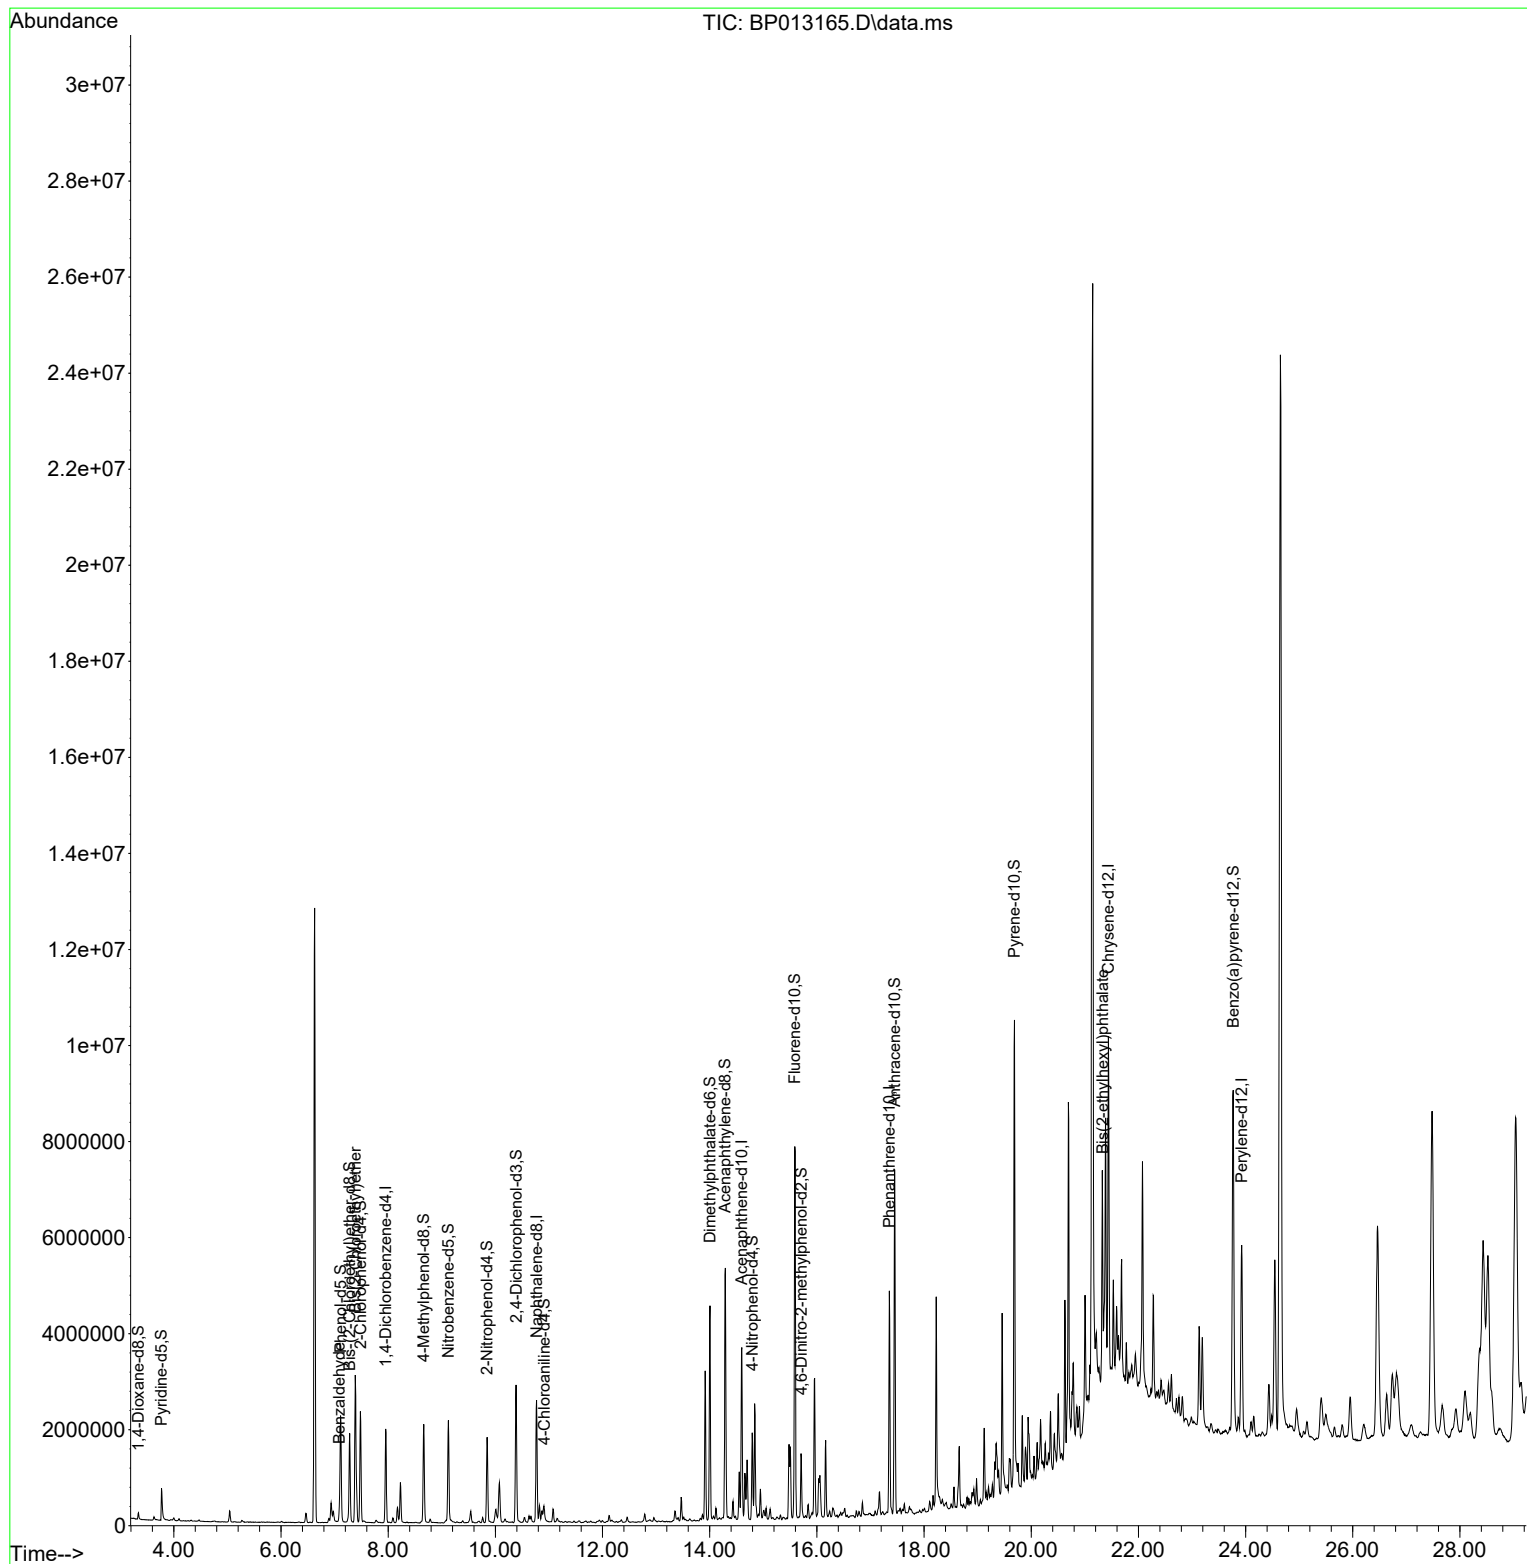


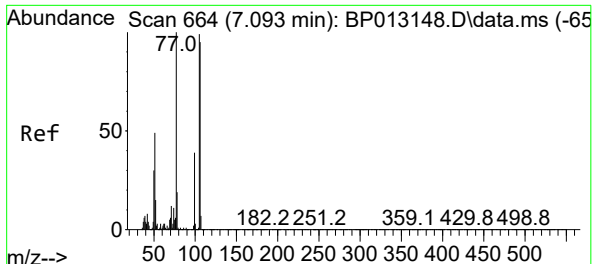

#6
Benzaldehyde
Concen: 4.885 ng/ul
RT: 7.087 min Scan# 610
Delta R.T. -0.006 min
Lab File: BP013165.D
Acq: 20 Dec 2022 14:12




Instrument :
BNA_P
ClientSampleId :
DBXQ8


Tgt Ion: 77 Resp: 82465
Ion Ratio Lower Upper
77 100
105 92.2 81.5 122.3
106 86.6 76.9 115.3

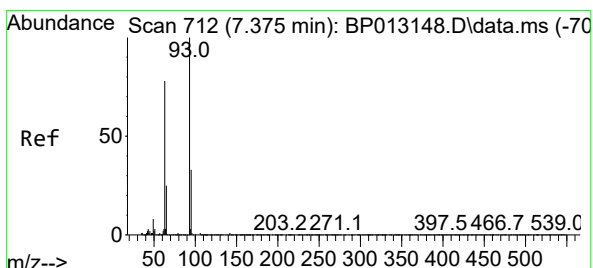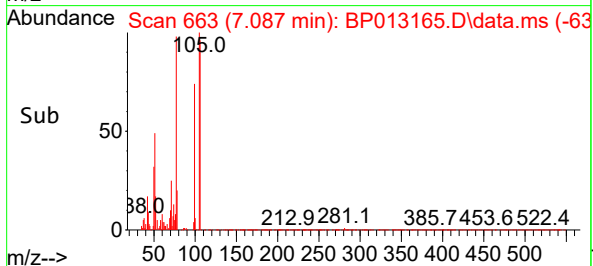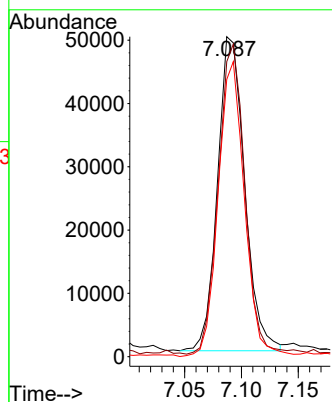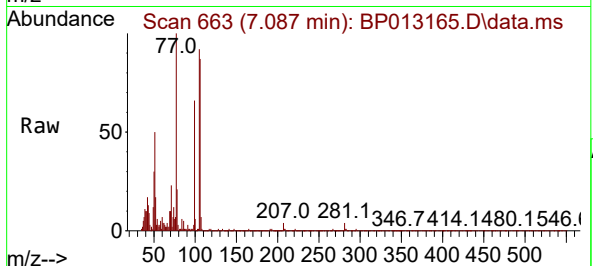

#10
Bis(2-Chloroethyl)ether
Concen: 35.415 ng/ul
RT: 7.387 min Scan# 714
Delta R.T. 0.012 min
Lab File: BP013165.D
Acq: 20 Dec 2022 14:12

Tgt Ion: 93 Resp: 1267106
Ion Ratio Lower Upper
93 100
63 2.2 59.8 89.8#
95 2.3 26.4 39.6#

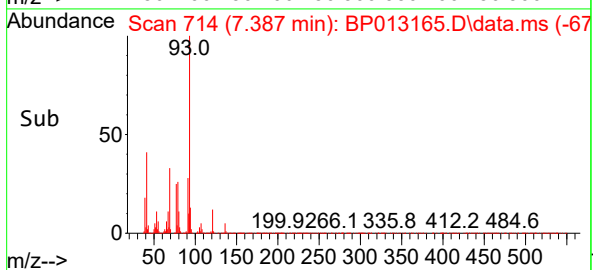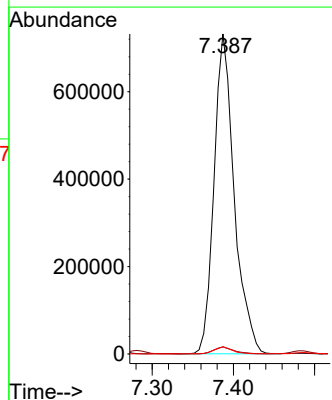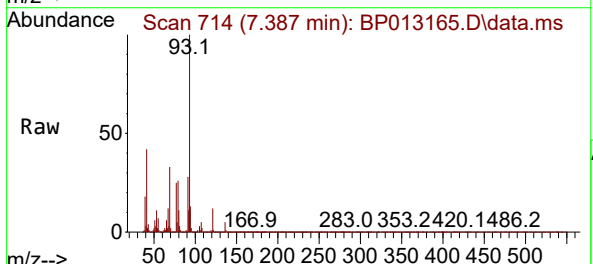

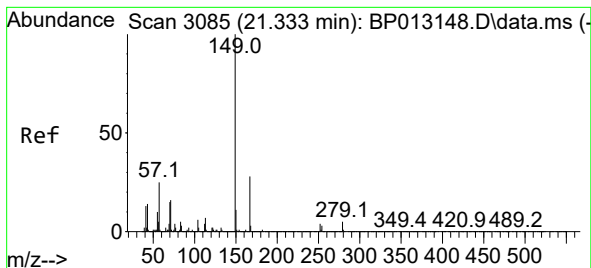

#86

Bis(2-ethylhexyl)phthalate

Concen: 1.150 ng/ul

RT: 21.333 min Scan# 3085

Delta R.T. 0.000 min

Lab File: BP013165.D


Acq: 20 Dec 2022 14:12

Instrument :

BNA_P

ClientSampleId :

DBXQ8

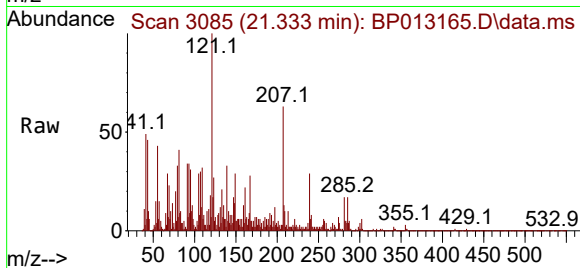

Tgt Ion:149 Resp: 119663

Ion Ratio Lower Upper

149 100

167 97.3 22.5 33.7#

279 3.0 3.8 5.8#

