

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013173.D
 Acq On : 20 Dec 2022 18:47
 Operator : CG/JU
 Sample : N6003-13
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXQ4

Quant Time: Dec 20 21:48:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	549377	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	2148265	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164	1254839	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	2658573	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2926109	20.000	ng/ul	0.00
88) Perylene-d12	23.921	264	3416906	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	105241	8.191	ng/uL	0.00
4) Pyridine-d5	3.764	84	1016824	27.858	ng/ul	0.00
7) Phenol-d5	7.116	99	1763780	39.416	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	1238373	45.876	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	1508629	42.827	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	258980	7.063	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	793434	50.269	ng/ul	0.00
24) 2-Nitrophenol-d4	9.846	143	913105	51.386	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1363442	39.503	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	391375	8.032	ng/ul	0.00
46) Dimethylphthalate-d6	14.004	166	4619159	47.897	ng/ul	0.00
49) Acenaphthylene-d8	14.293	160	5281513	49.839	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	684273	39.445	ng/ul	0.00
60) Fluorene-d10	15.592	176	3957636	48.507	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	637637	37.270	ng/ul	0.00
73) Anthracene-d10	17.451	188	5700485	47.528	ng/ul	0.00
81) Pyrene-d10	19.686	212	7702577	45.860	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	8281922	48.628	ng/ul	0.00
Target Compounds					Qvalue	
6) Benzaldehyde	7.087	77	17626	1.006	ng/ul	87
10) Bis(2-Chloroethyl)ether	7.387	93	770617	20.752	ng/ul#	24
86) Bis(2-ethylhexyl)phtha...	21.333	149	115479	1.078	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013173.D
Acq On : 20 Dec 2022 18:47
Operator : CG/JU
Sample : N6003-13
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXQ4

Quant Time: Dec 20 21:48:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration




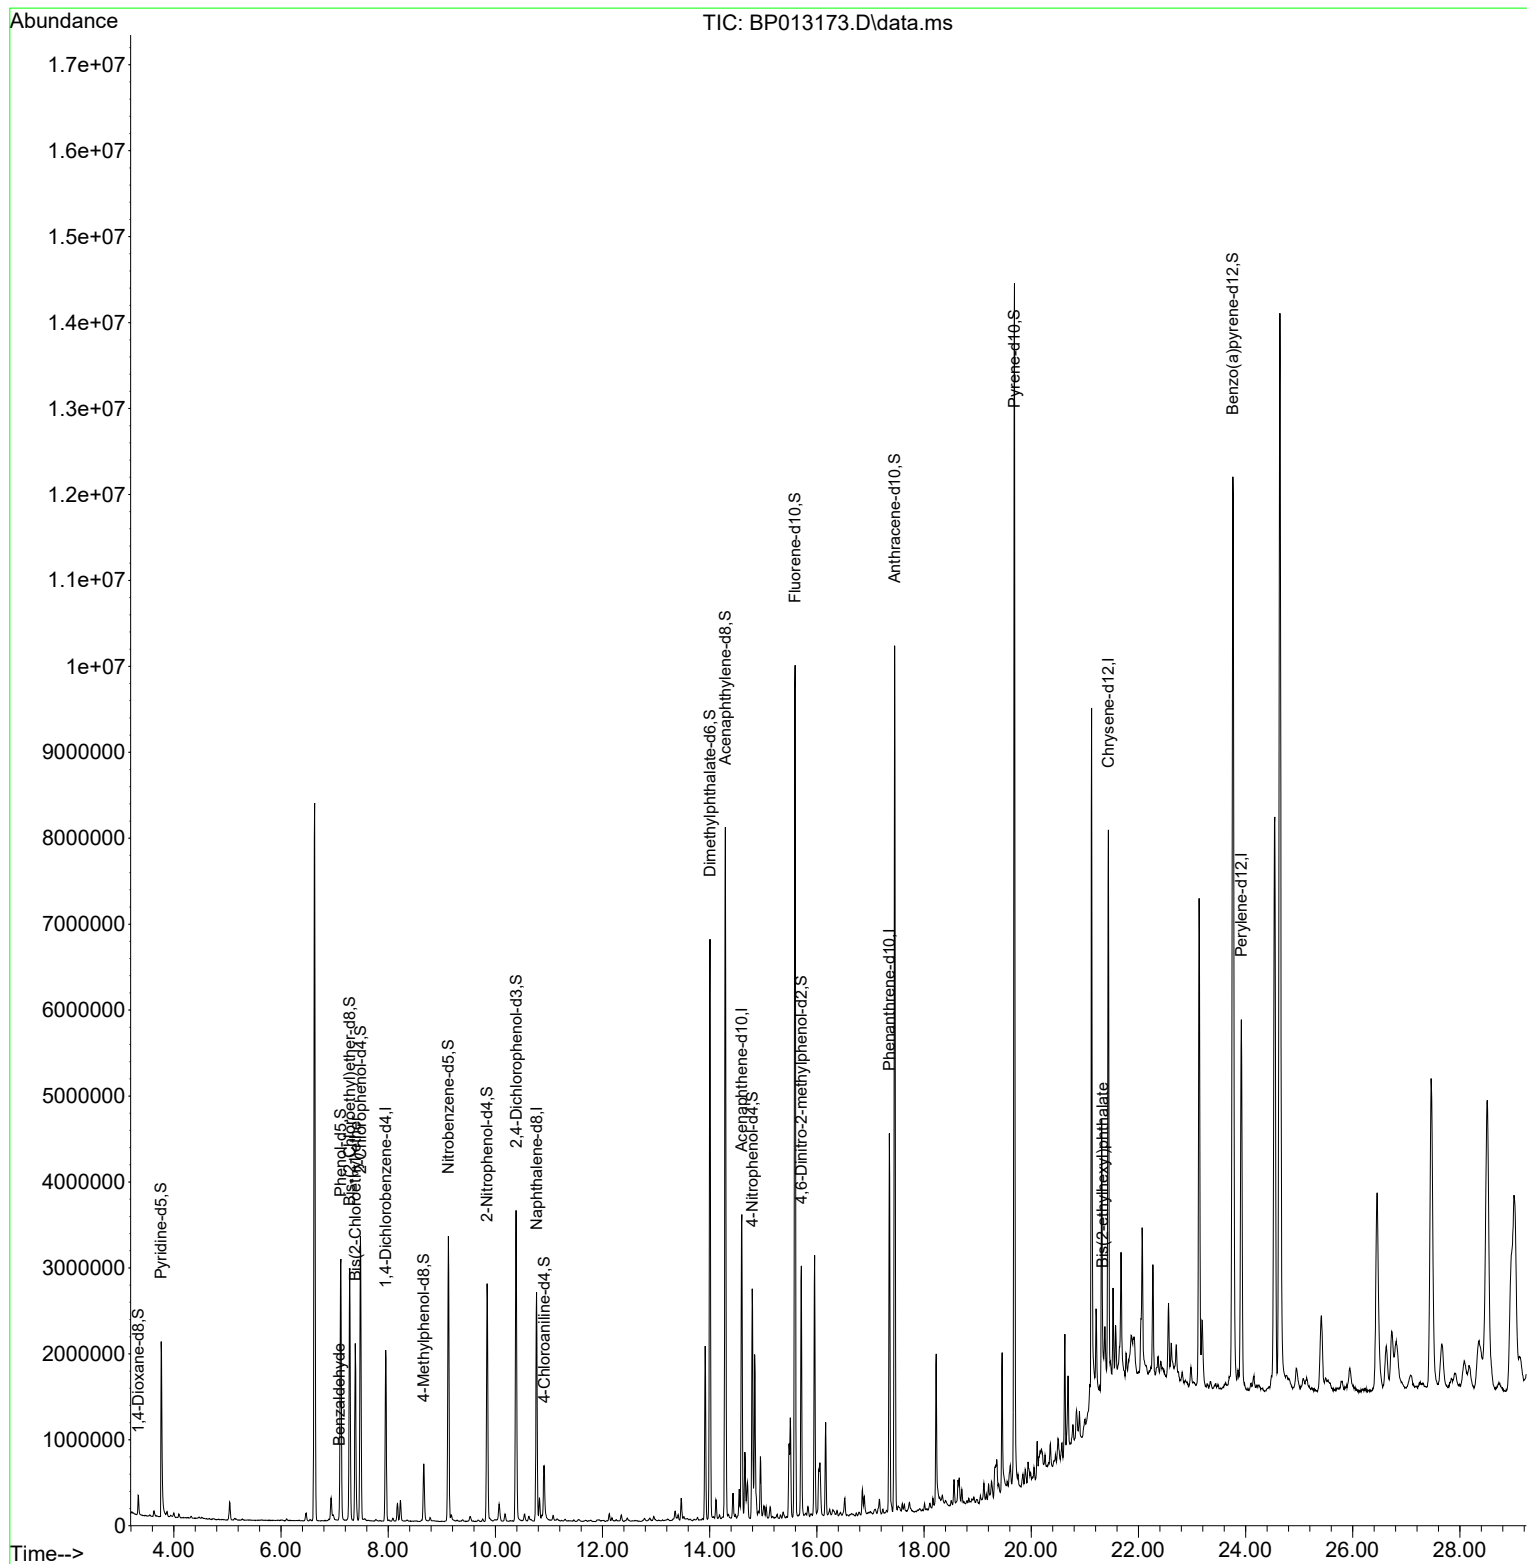


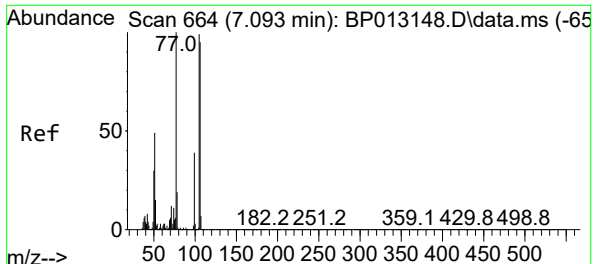

#6
Benzaldehyde
Concen: 1.006 ng/ul
RT: 7.087 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP013173.D
Acq: 20 Dec 2022 18:47




Instrument :
BNA_P
ClientSampleId :
DBXQ4


Tgt Ion: 77 Resp: 17626
Ion Ratio Lower Upper
77 100
105 91.7 81.5 122.3
106 79.8 76.9 115.3

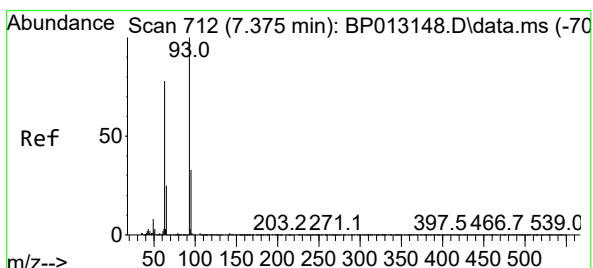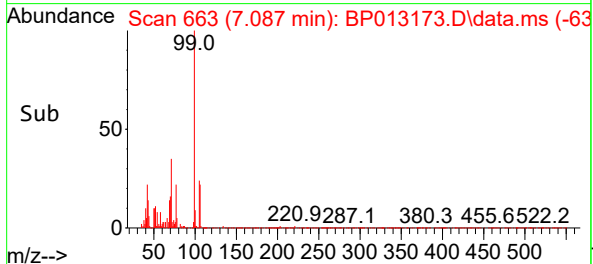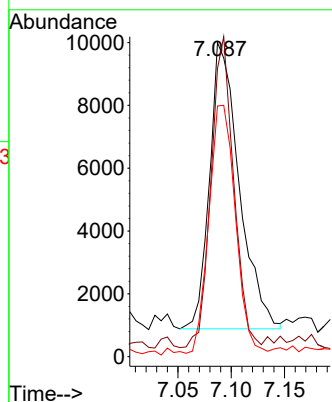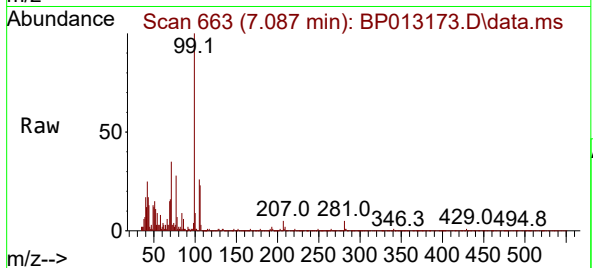

#10
Bis(2-Chloroethyl)ether
Concen: 20.752 ng/ul
RT: 7.387 min Scan# 714
Delta R.T. 0.012 min
Lab File: BP013173.D
Acq: 20 Dec 2022 18:47

Tgt Ion: 93 Resp: 770617
Ion Ratio Lower Upper
93 100
63 2.0 59.8 89.8#
95 2.3 26.4 39.6#

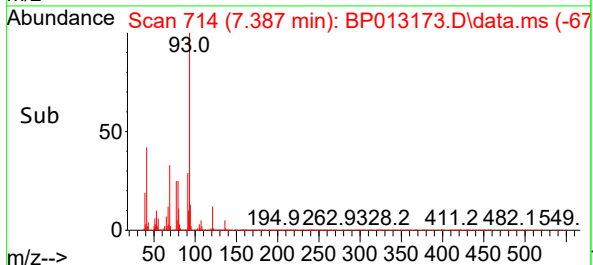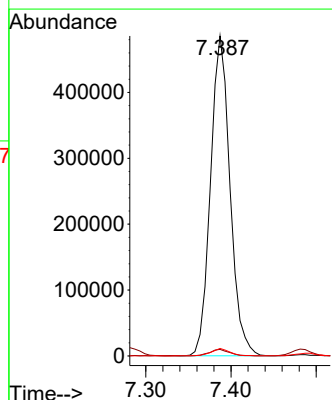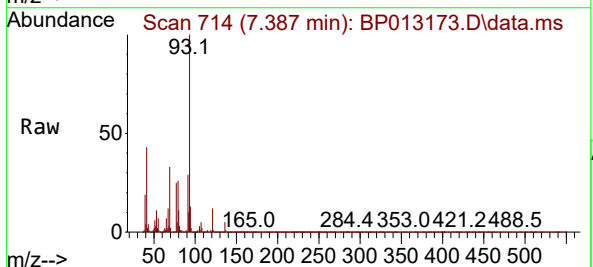

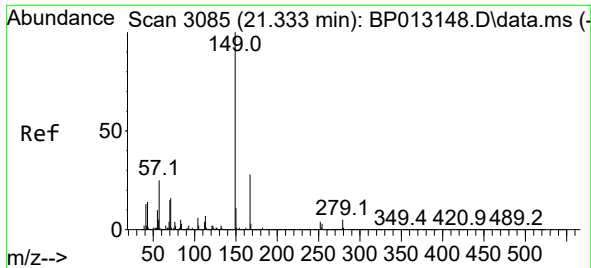

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.078 ng/ul
 RT: 21.333 min Scan# 3085
 Delta R.T. 0.000 min
 Lab File: BP013173.D
 Acq: 20 Dec 2022 18:47

Instrument :
 BNA_P
 ClientSampleId :
 DBXQ4

Tgt Ion:149 Resp: 115479
 Ion Ratio Lower Upper
 149 100
 167 42.6 22.5 33.7#
 279 4.7 3.8 5.8

