




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013225.D
 Acq On : 22 Dec 2022 01:27
 Operator : CG/JU
 Sample : N6032-08
 Misc :
 ALS Vial : 108 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA0

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:20:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

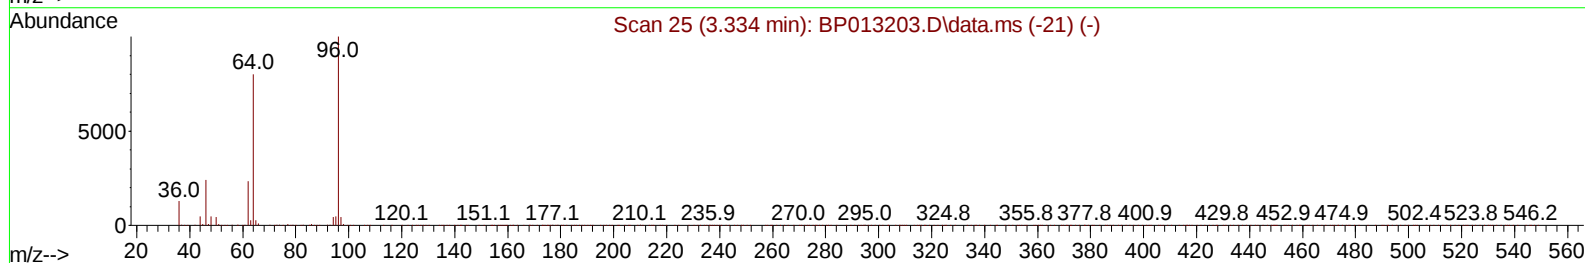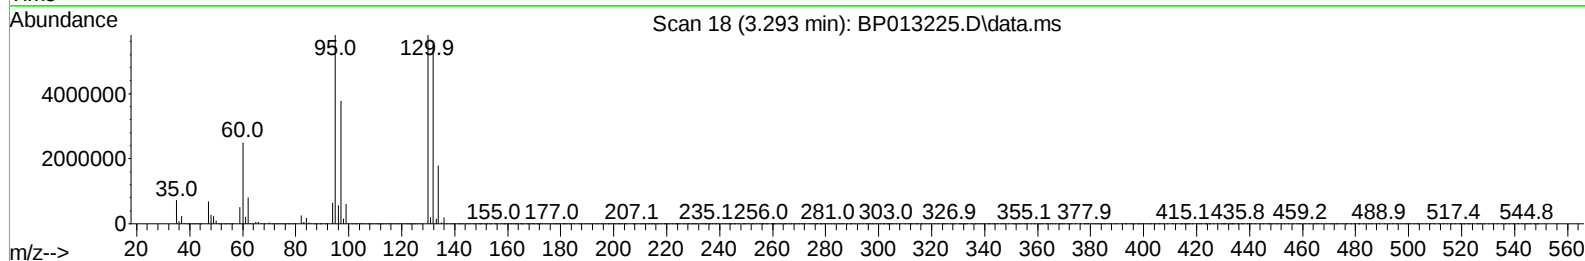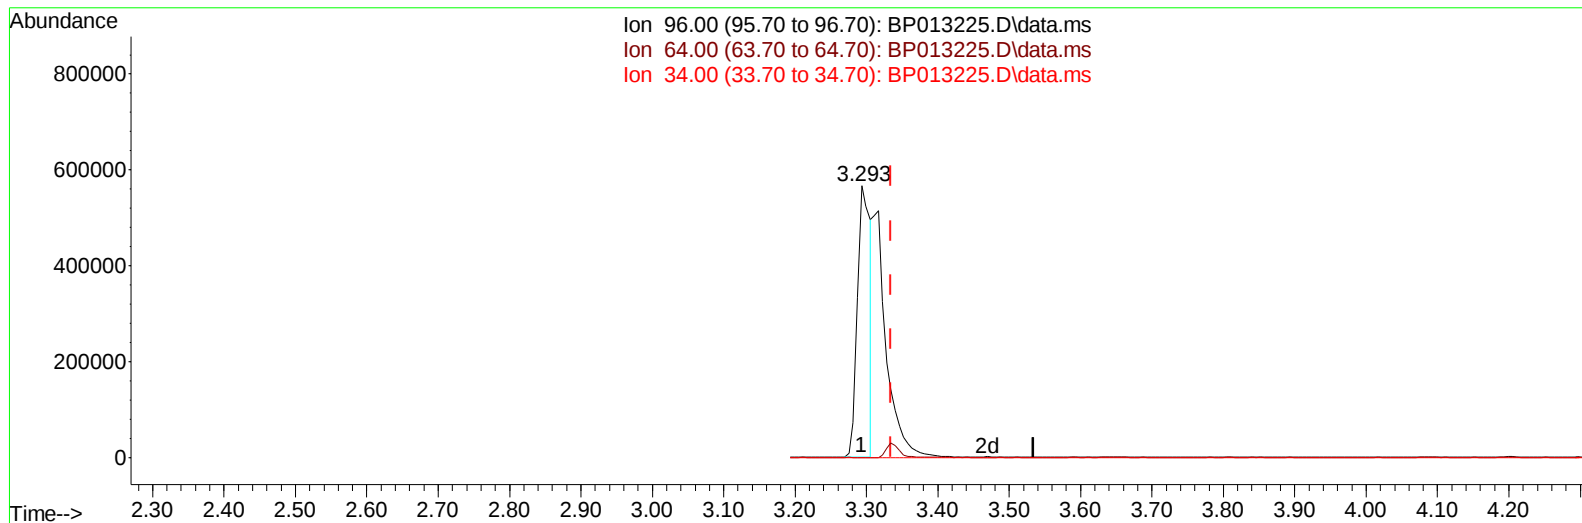

TIC: BP013225.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.041) 61.77 ng/uL

response 705064

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013225.D
 Acq On : 22 Dec 2022 01:27
 Operator : CG/JU
 Sample : N6032-08
 Misc :
 ALS Vial : 108 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA0

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:20:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

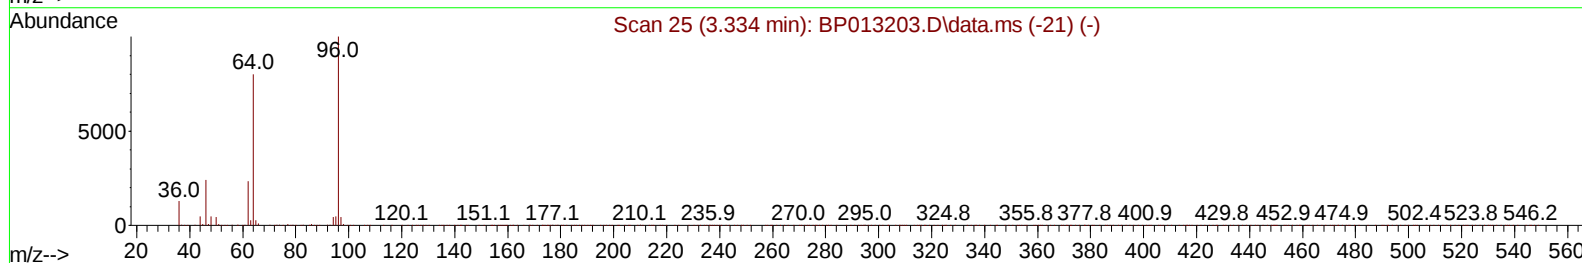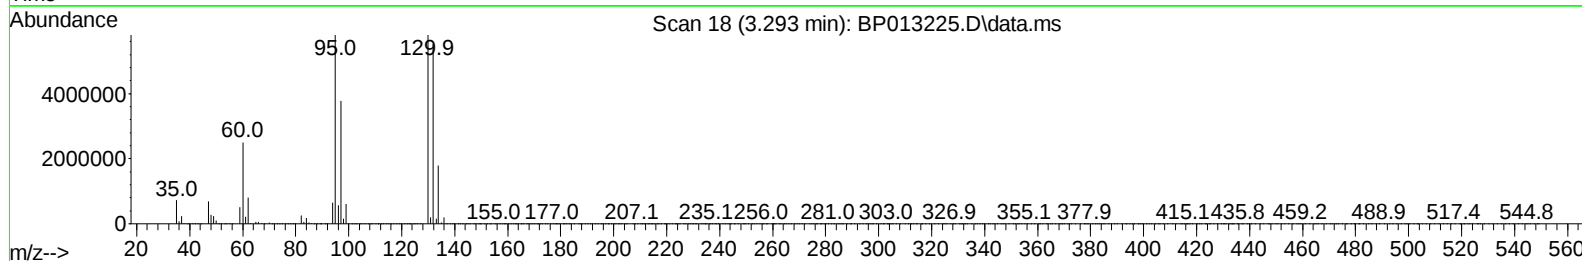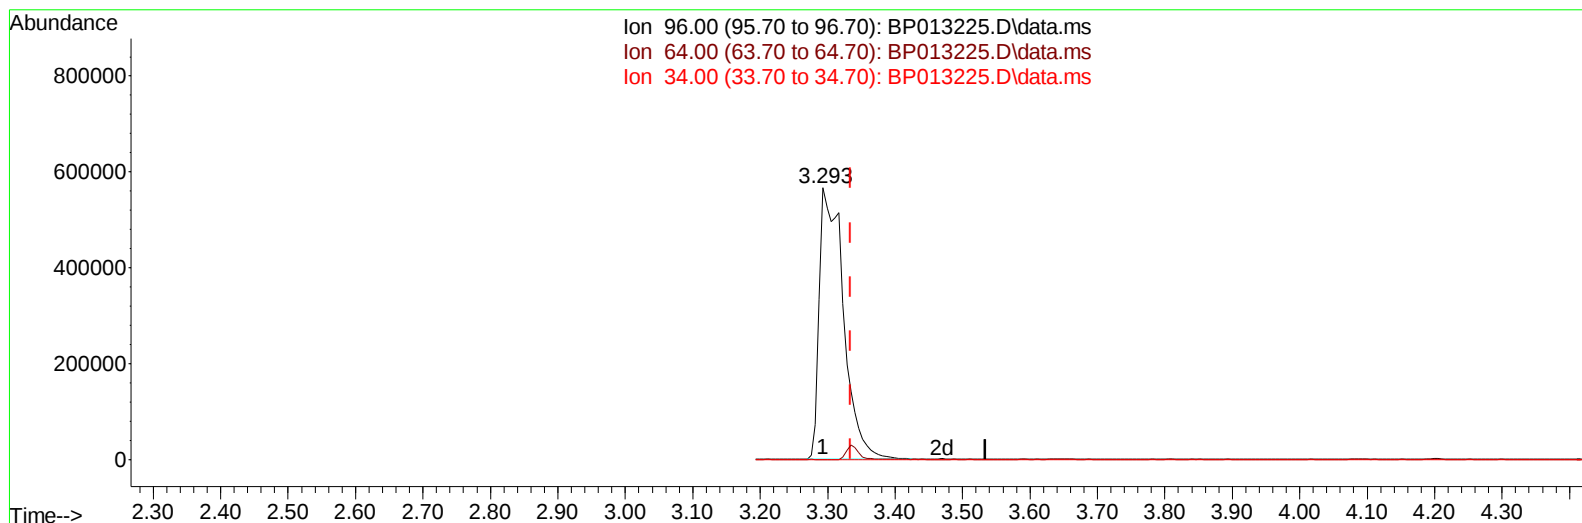

TIC: BP013225.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.041) 123.05 ng/uL m

response 1404528

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013225.D
 Acq On : 22 Dec 2022 01:27
 Operator : CG/JU
 Sample : N6032-08
 Misc :
 ALS Vial : 108 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA0

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:20:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	488037	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	1965191	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1109004	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2064324	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2058730	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	2422081	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1404528m	123.050	ng/uL	-0.04
4) Pyridine-d5	3.781	84	69117	2.132	ng/ul	0.02
7) Phenol-d5	7.105	99	284368	7.154	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	787328	32.833	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	669788	21.404	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	441200	13.546	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	497514	34.457	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	465766	28.653	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	792218	25.091	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	328842	7.378	ng/ul	0.00
46) Dimethylphthalate-d6	13.999	166	2814494	33.022	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	3216212	34.341	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	51798	3.379	ng/ul	0.00
60) Fluorene-d10	15.587	176	2433075	33.743	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	272993	20.550	ng/ul	0.00
73) Anthracene-d10	17.445	188	3572807	38.363	ng/ul	0.00
81) Pyrene-d10	19.675	212	4204381	35.579	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	4654910	38.558	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013225.D
Acq On : 22 Dec 2022 01:27
Operator : CG/JU
Sample : N6032-08
Misc :
ALS Vial : 108 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLA0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/22/2022
Supervised By :mohammad ahmed 12/22/2022

Quant Time: Dec 22 05:20:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 23:38:37 2022
Response via : Initial Calibration

