




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013226.D
 Acq On : 22 Dec 2022 02:01
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA1

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:23:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

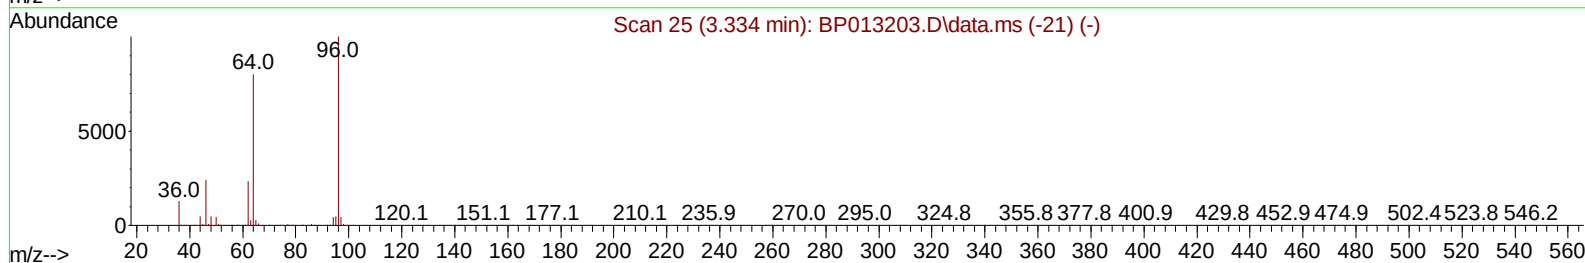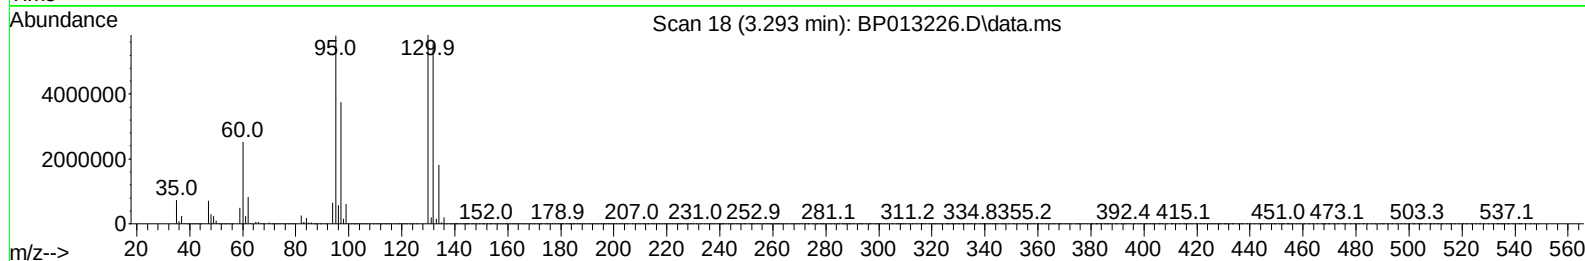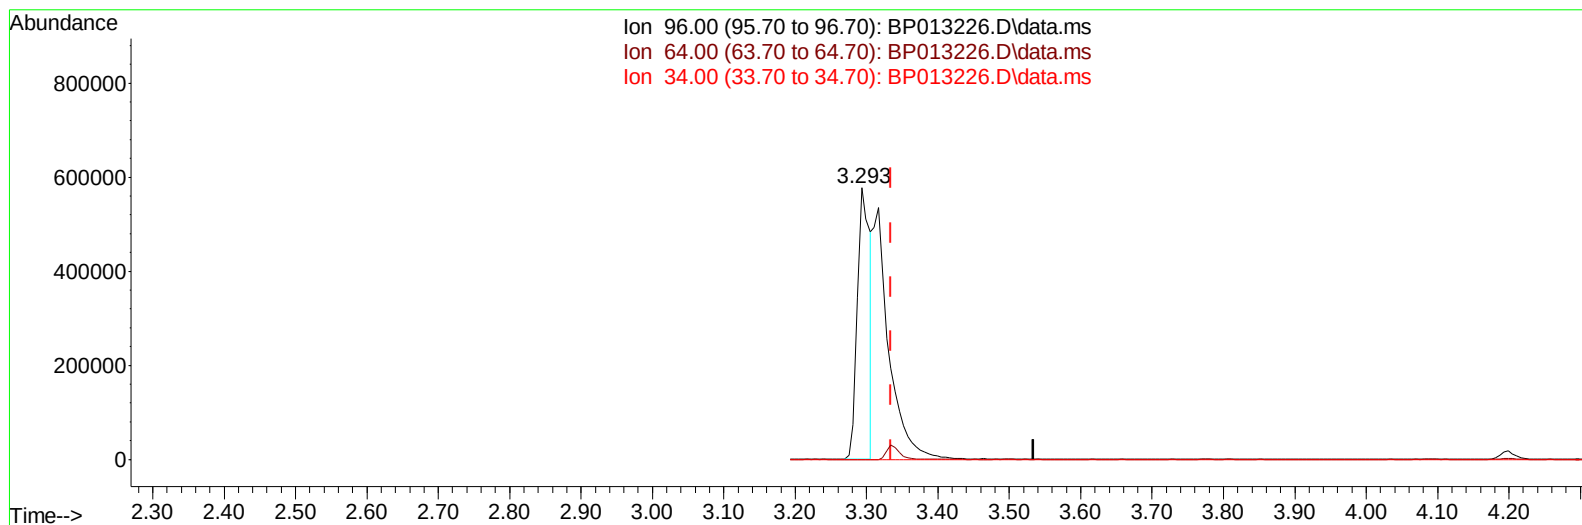

TIC: BP013226.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.041) 61.60 ng/uL

response 703570

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013226.D
 Acq On : 22 Dec 2022 02:01
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA1

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:23:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

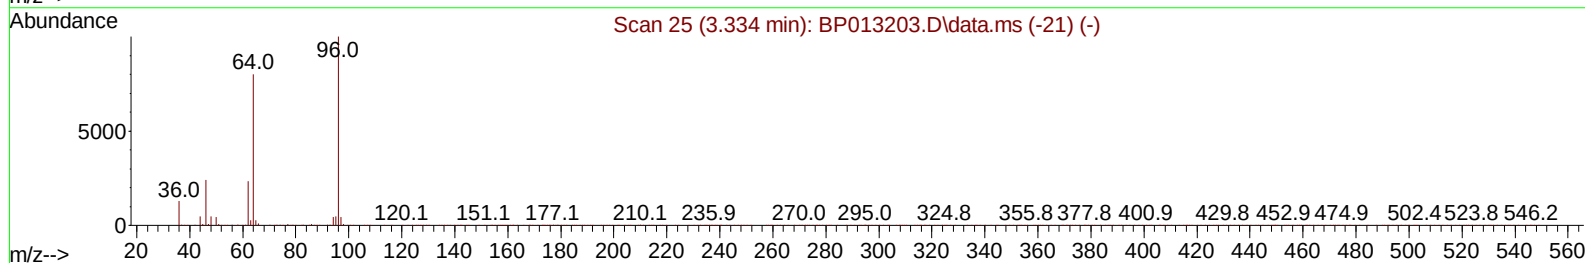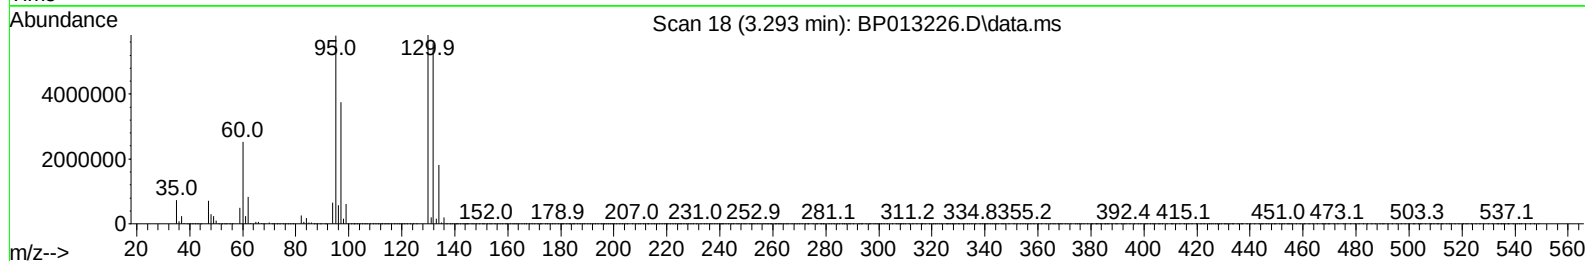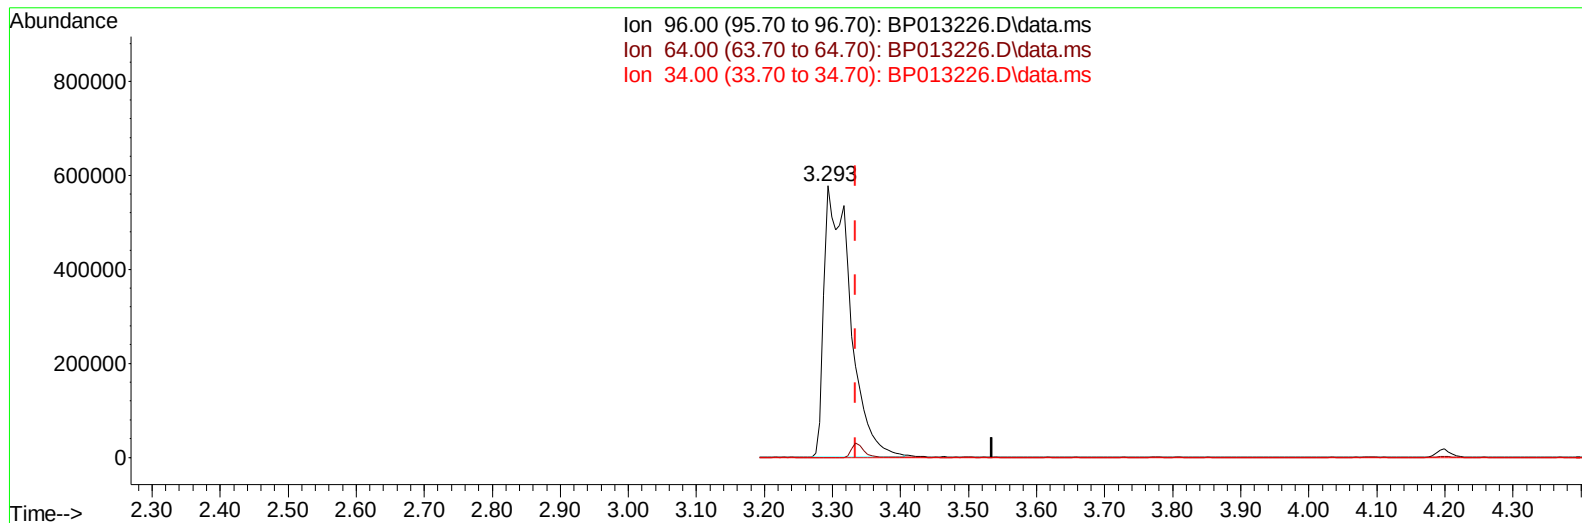

TIC: BP013226.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.293min (-0.041) 135.10 ng/uL m

response 1542895

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013226.D
 Acq On : 22 Dec 2022 02:01
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 109 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COLA1

Manual IntegrationsAPPROVED

Quant Time: Dec 22 05:23:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 21 23:38:37 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	488315	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	1900712	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	1061128	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2077570	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	2197820	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	2616434	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	1542895m	135.095	ng/uL	-0.04
4) Pyridine-d5	3.781	84	64276	1.981	ng/ul	0.02
7) Phenol-d5	7.105	99	268967	6.762	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	780394	32.525	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	668819	21.361	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	430321	13.204	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	478263	34.247	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	461783	29.372	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	765602	25.071	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	480267	11.140	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	2581201	31.651	ng/ul	0.00
49) Acenaphthylene-d8	14.287	160	3060894	34.157	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	46779	3.189	ng/ul	0.00
60) Fluorene-d10	15.581	176	2304894	33.407	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	259906	19.440	ng/ul	0.00
73) Anthracene-d10	17.445	188	3528496	37.646	ng/ul	0.00
81) Pyrene-d10	19.675	212	4417042	35.013	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.745	264	4801293	36.816	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013226.D
Acq On : 22 Dec 2022 02:01
Operator : CG/JU
Sample : N6032-09
Misc :
ALS Vial : 109 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COLA1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/22/2022
Supervised By :mohammad ahmed 12/22/2022

Quant Time: Dec 22 05:23:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 21 23:38:37 2022
Response via : Initial Calibration

