

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013144.D
 Acq On : 20 Dec 2022 01:10
 Operator : CG/JU
 Sample : N6006-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXV6

Quant Time: Dec 20 02:32:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	580239	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	2424287	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	1500673	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	2958683	20.000	ng/u1	0.00
79) Chrysene-d12	21.433	240	2179413	20.000	ng/u1	0.00
88) Perylene-d12	23.916	264	2608957	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	72209	5.321	ng/uL	0.00
4) Pyridine-d5	3.770	84	435444	11.296	ng/u1	0.00
7) Phenol-d5	7.111	99	1423862	30.127	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	924958	32.443	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	1193894	32.090	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	1008246	26.036	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	608730	34.176	ng/u1	0.00
24) 2-Nitrophenol-d4	9.846	143	703797	35.097	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1258166	32.302	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	989975	18.004	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	3759243	32.595	ng/u1	0.00
49) Acenaphthylene-d8	14.293	160	4258841	33.605	ng/u1	0.00
54) 4-Nitrophenol-d4	14.793	143	459634	22.155	ng/u1	0.00
60) Fluorene-d10	15.587	176	3171004	32.499	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	502137	26.373	ng/u1	0.00
73) Anthracene-d10	17.451	188	4353085	32.612	ng/u1	0.00
81) Pyrene-d10	19.680	212	4502353	35.991	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	4243514	32.632	ng/u1	0.00
Target Compounds						
80) Fluoranthene	19.357	202	150811	1.062	ng/u1#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013144.D
Acq On : 20 Dec 2022 01:10
Operator : CG/JU
Sample : N6006-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXV6

Quant Time: Dec 20 02:32:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

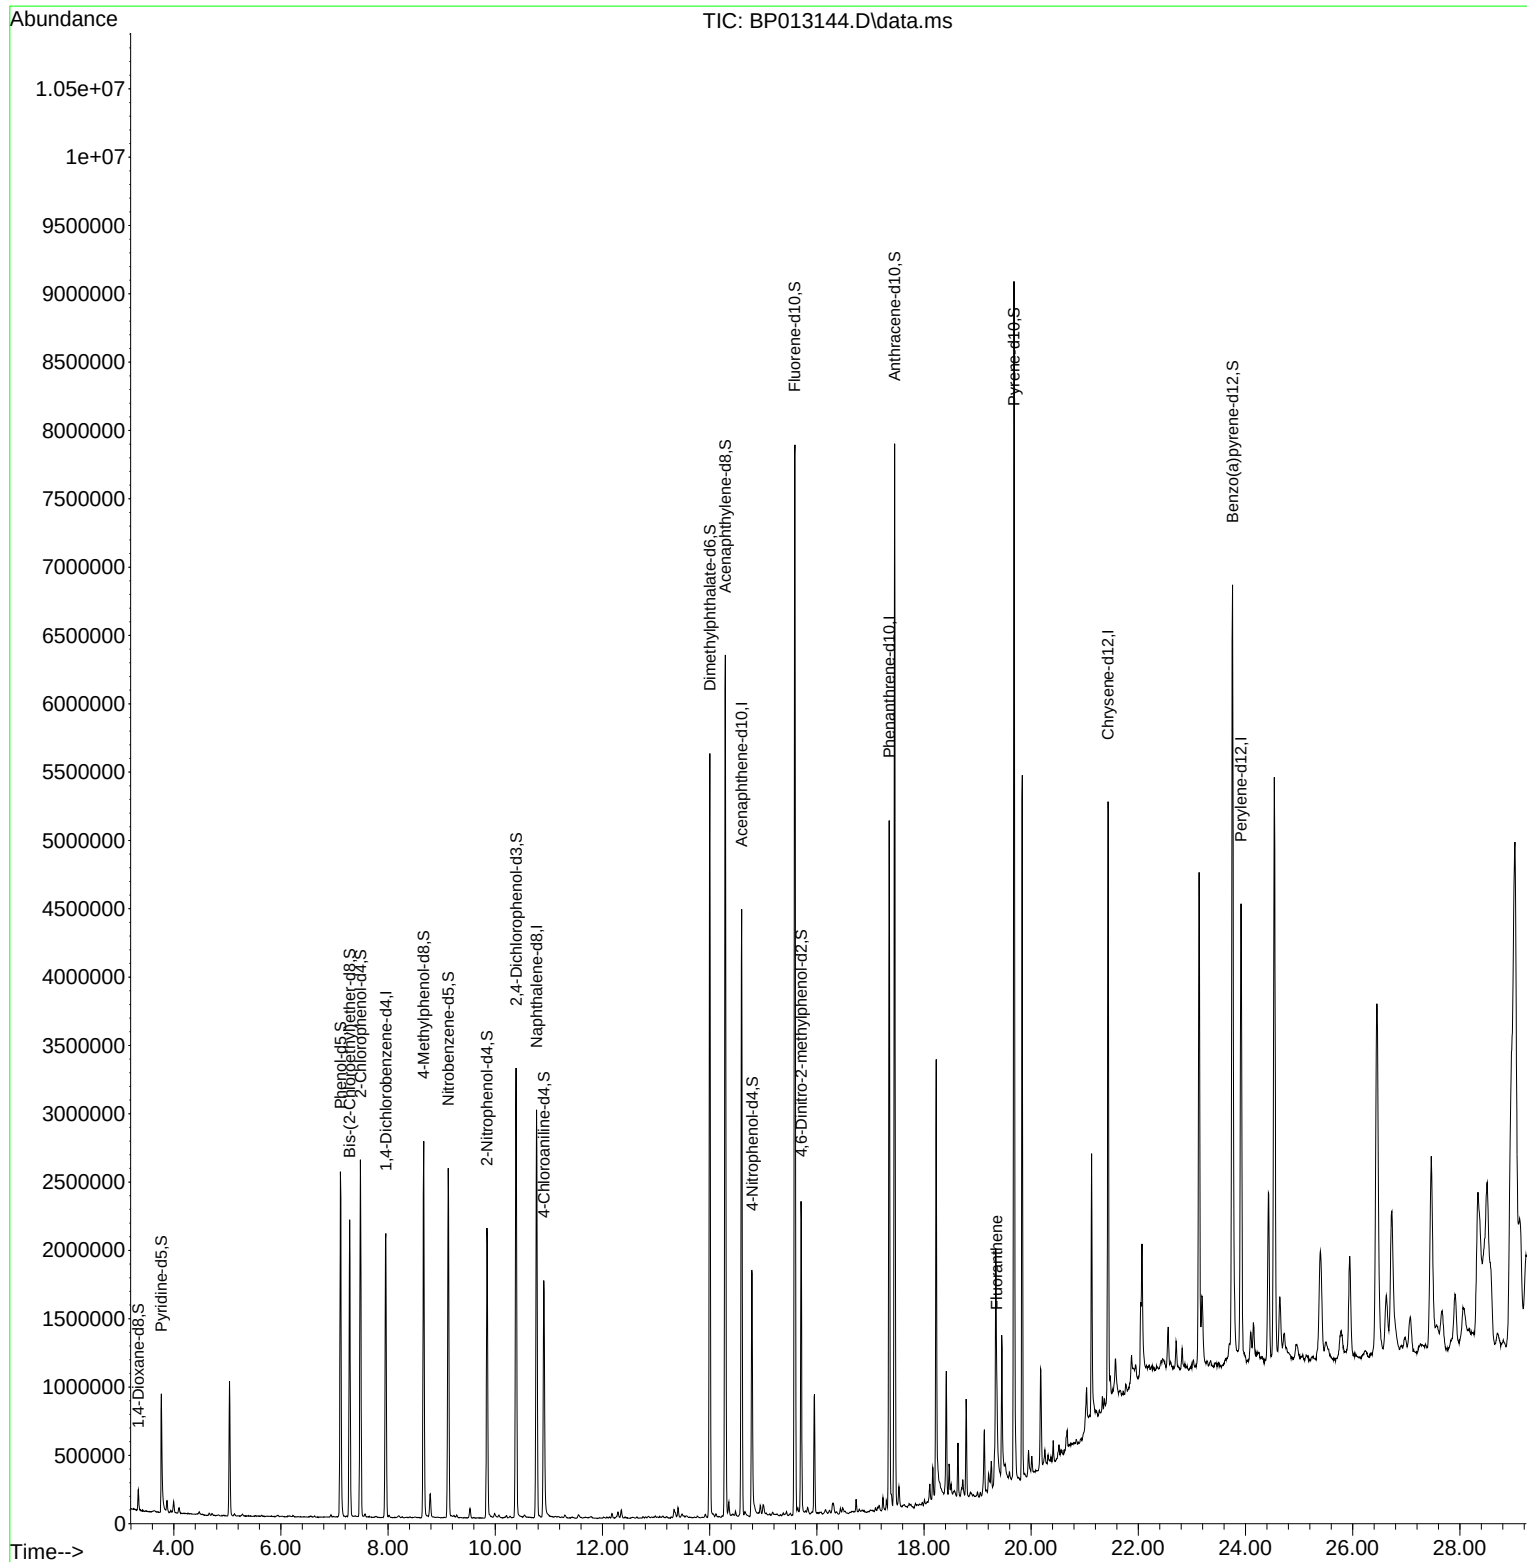

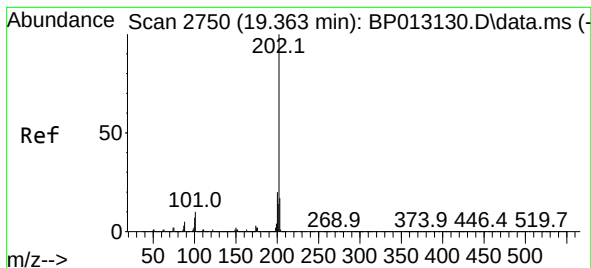

#80
 Fluoranthene
 Concen: 1.062 ng/ul
 RT: 19.357 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP013144.D
 Acq: 20 Dec 2022 01:10

Instrument :
 BNA_P
 ClientSampleId :
 DBXV6

Tgt Ion:202 Resp: 150811
 Ion Ratio Lower Upper
 202 100
 101 12.8 8.2 12.2#
 100 8.8 6.1 9.1

