

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
 Data File : BP013163.D
 Acq On : 20 Dec 2022 13:04
 Operator : CG/JU
 Sample : N6003-13
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXQ4

Quant Time: Dec 20 21:45:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 19 21:43:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	499103	20.000	ng/u1	0.00
20) Naphthalene-d8	10.769	136	1878369	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	1028254	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.351	188	2126917	20.000	ng/u1	0.00
79) Chrysene-d12	21.439	240	2326007	20.000	ng/u1	0.00
88) Perylene-d12	23.921	264	2725166	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	113443	9.718	ng/uL	0.00
4) Pyridine-d5	3.764	84	1086271	32.759	ng/u1	0.00
7) Phenol-d5	7.111	99	1845866	45.405	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67	1301290	53.063	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	1594572	49.826	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	291643	8.755	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	827725	59.976	ng/u1	0.00
24) 2-Nitrophenol-d4	9.846	143	940926	60.560	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	1388906	46.023	ng/u1	0.00
31) 4-Chloroaniline-d4	10.910	131	422791	9.924	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	4407954	55.779	ng/u1	0.00
49) Acenaphthylene-d8	14.293	160	5172218	59.563	ng/u1	0.00
54) 4-Nitrophenol-d4	14.792	143	658391	46.316	ng/u1	0.00
60) Fluorene-d10	15.592	176	3795207	56.767	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	617737	45.133	ng/u1	0.00
73) Anthracene-d10	17.451	188	5453273	56.832	ng/u1	0.00
81) Pyrene-d10	19.686	212	7386794	55.327	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.763	264	7953705	58.555	ng/u1	0.00
Target Compounds						
90) Benzo(b)fluoranthene	23.163	252	175498	1.010	ng/u1#	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121922\
Data File : BP013163.D
Acq On : 20 Dec 2022 13:04
Operator : CG/JU
Sample : N6003-13
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXQ4

Quant Time: Dec 20 21:45:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 19 21:43:11 2022
Response via : Initial Calibration

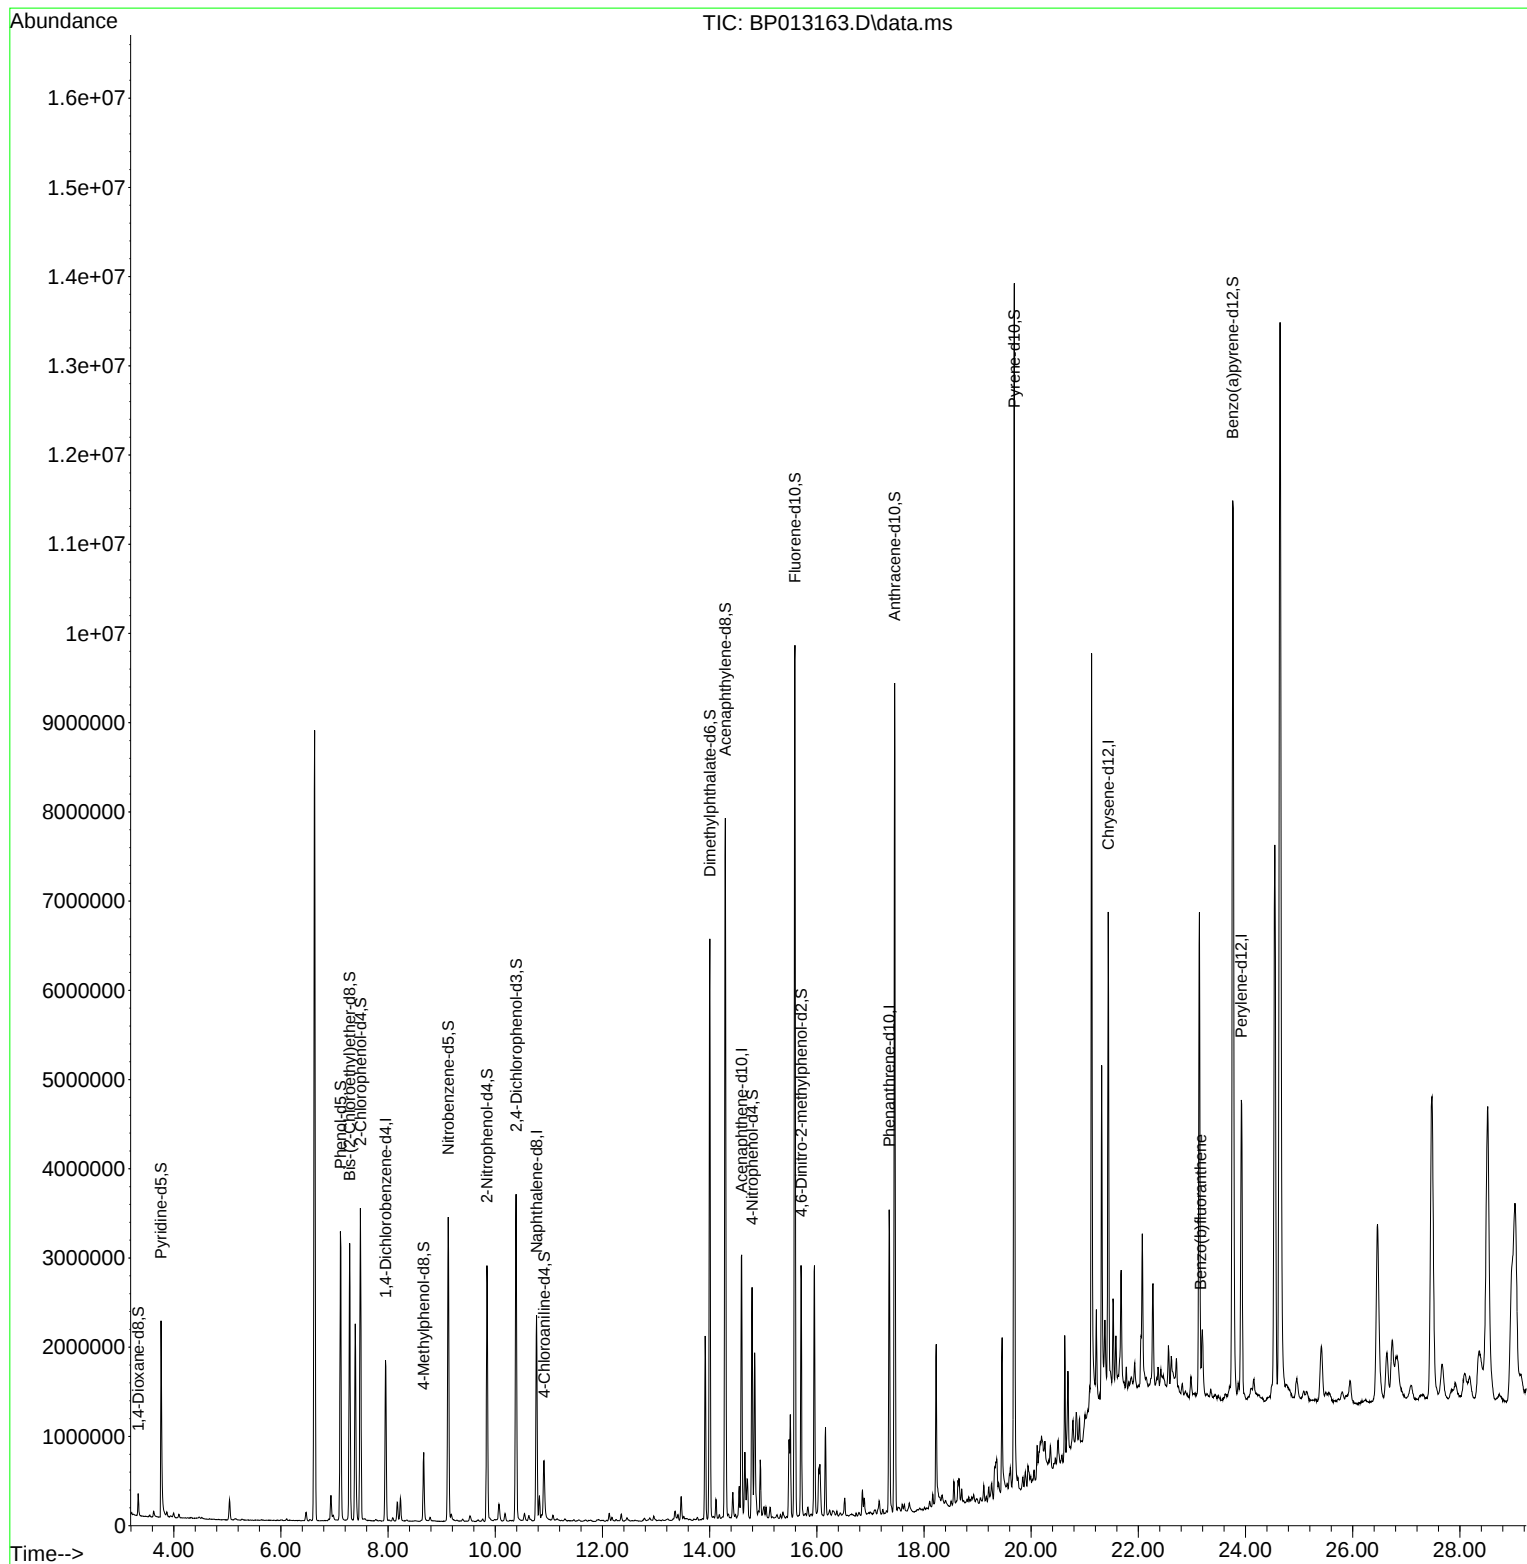

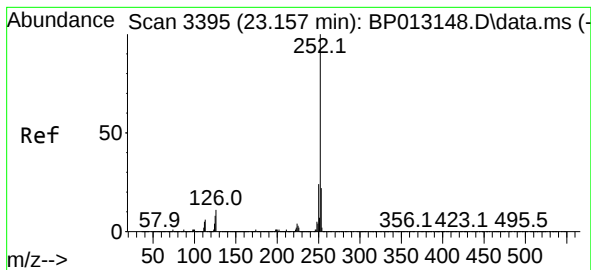

#90

Benzo(b)fluoranthene

Concen: 1.010 ng/ul

RT: 23.163 min Scan# 33

Delta R.T. 0.000 min

Lab File: BP013163.D


Acq: 20 Dec 2022 13:04

Instrument :

BNA_P

ClientSampleId :

DBXQ4

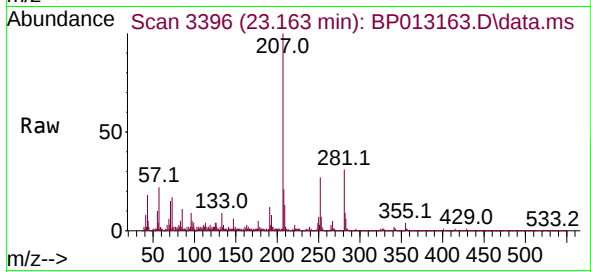

Tgt Ion:252 Resp: 175498

Ion Ratio Lower Upper

252 100

253 25.6 17.7 26.5

125 14.9 6.8 10.2#

